



US MEDICAL TECHNOLOGY INDUSTRY

2019 MARKET STUDY



Imprint

Author

German American Chamber of Commerce, Inc. (AHK USA-New York)
80 Pine Street, 24th Floor
New York, NY 10005
Phone: +1 (212) 974-8830 | Fax: +1 (212) 974-8867
Email: info@gaccny.com | Web: www.gaccny.com

As of January 31, 2019

Contact

Dr. Jens Daum, legalservices@gaccny.com
Nicole Klug, consulting@gaccny.com

Editors

Nicole Klug, AHK USA-New York
Natalie Wittmann, AHK USA-New York
Leonhard Römisch, AHK USA-New York
Eva Weik, AHK USA-New York

Disclaimer

Please note that the German American Chamber of Commerce, Inc. New York (AHK USA-New York) is a company under U.S. law that provides information on German-American trade in return for expense-based compensation. This does not constitute binding legal advice. Rather, we offer general consultation services, for the correctness of which no liability can be assumed in terms of content.

All content was created with the greatest possible care and to the best of our knowledge. Conducted interviews are the opinion of respondents and do not necessarily reflect the opinion of the publisher. Our offer contains links to external websites of third parties whose content we have no influence on. For the content of linked pages, the respective provider or operator of said pages is always responsible and the AHK USA-New York assumes no liability. To the extent that personal data (for example names, addresses or email addresses) are collected on our website, this is done on a voluntary basis and / or can be researched online. The publisher assumes no responsibility for the topicality, correctness, completeness or quality of the information provided.

For damage of a material or immaterial nature caused directly or indirectly by the use or non-use of information provided, the publisher shall not be liable, unless there is evidence of willful intent or gross negligence on the part of the publisher.

Copyright

This market study and its content is copyright of [the MAGIA – MedTech Alliance for Global Internationalisation projects team, Lyonbiote, BioWin, Bioindustry Park Silvano Fumero SpA / bioPmed, Life Science Nord] - © [MAGIA project team] [2019]. All rights reserved.

Any redistribution or reproduction of part or all of the content in any form is prohibited other than the following:

- you may print or download to a local hard disk the study for your personal and non-commercial use only
- you may copy the content to individual third parties for their personal use, but only if you acknowledge the MAGIA project as the source of the material

You may not, except with our express written permission, distribute, publish or commercially exploit the content. Nor may you transmit it or store it on any other website or other form of electronic retrieval system.

Table of Contents

1. GENERAL MARKET OVERVIEW.....	6
1.1. AN INTRODUCTION TO THE US MEDICAL TECHNOLOGY INDUSTRY.....	7
1.1.1. EXPORT AND IMPORT OF MEDICAL DEVICES.....	8
1.1.2. ECONOMIES OF SCALE.....	12
1.1.3. MARKETS FOR MEDICAL TECHNOLOGY.....	13
1.1.4. EXTERNAL DRIVERS.....	14
1.1.5. ECONOMIC GROWTH OF MEDICAL TECHNOLOGY BY REGION.....	15
1.1.6. MEDICAL DEVICE COMPANIES AND KEY DISTRIBUTORS.....	17
1.1.7. PROFILE OF THE TOP THREE US MEDICAL TECHNOLOGY COMPANIES.....	17
1.1.8. KEY DISTRIBUTORS (GROUP PURCHASING ORGANIZATIONS).....	19
1.1.9. RESEARCH AND DEVELOPMENT.....	20
1.2. CARDIOVASCULAR.....	22
1.2.1. MEDICAL TECHNOLOGICAL MARKET FOR CARDIOVASCULAR DISEASES.....	22
1.2.1.1. MARKET SIZE & GROWTH.....	22
1.2.1.2. US COMPANIES FOR CARDIOVASCULAR.....	22
1.2.2. ASSOCIATIONS FOR CARDIOVASCULAR DISEASES.....	25
1.3. DENTISTRY.....	26
1.3.1. MEDICAL TECHNOLOGICAL MARKET FOR DENTISTRY.....	26
1.3.1.1. MARKET SIZE & GROWTH.....	26
1.3.1.2. US COMPANIES FOR DENTISTRY.....	28
1.3.2. ASSOCIATIONS FOR DENTAL EQUIPMENT.....	30
1.4. ONCOLOGY.....	30
1.4.1. MEDICAL TECHNOLOGICAL MARKET FOR ONCOLOGY.....	30
1.4.1.1. MARKET SIZE & GROWTH.....	31
1.4.1.2. US COMPANIES FOR ONCOLOGY.....	31
1.4.2. ASSOCIATIONS.....	33
1.5. ORTHOPEDICS.....	34
1.5.1. MEDICAL TECHNOLOGICAL MARKET FOR ORTHOPEDICS.....	34
1.5.1.1. MARKET SIZE & GROWTH.....	35
1.5.1.2. US COMPANIES FOR ORTHOPEDICS.....	36
1.5.2. ASSOCIATIONS FOR ORTHOPEDIC.....	38

2. REGULATORY AFFAIRS40

2.1. US IMPORT REGULATION; GENERAL OVERVIEW40

- 2.1.1. TRADE POLICY FRAME WORK 40
- 2.1.2. CUSTOMS PROCEDURE..... 40
- 2.1.3. IMPORT DUTIES 41
- 2.1.4. IMPORT BANS & RESTRICTIONS..... 41
- 2.1.5. EXCURSE: EXPORT RESTRICTION (EU) 41

2.2. IMPORT OF MEDICAL DEVICES; SPECIFIC REGULATIONS42

- 2.2.1. FDA'S MEDICAL DEVICE REGULATION 42
- 2.2.2. SUPPLEMENTING & DISPLACED REGULATIONS..... 52

2.3. MEDICAL DEVICE REIMBURSEMENT54

- 2.3.1. SUNSHINE ACT..... 54
- 2.3.2. COVERAGE, CODING AND PAYMENT..... 55
- 2.3.3. CENTERS FOR MEDICARE & MEDICAID SERVICES (CMS)..... 56

3. MARKET ACCESS58

3.1. MARKET OPPORTUNITIES FOR FOREIGN COMPANIES IN THE US-MEDTECH

INDUSTRY58

3.2. MARKET BARRIERS.....59

3.3. SALES STRUCTURE AND MARKET ENTRY STRATEGIES61

- 3.3.1. SALES CHANNELS..... 62
- 3.3.2. PRESENCE IN THE USA..... 64

Table of Figures

FIGURE 1: TOTAL REVENUES OF US AND EUROPEAN MEDICAL TECHNOLOGY COMPANIES	8
FIGURE 2: IMPORTS	10
FIGURE 3: EXPORTS.....	10
FIGURE 4: PRODUCTS AND SERVICE SEGMENTATION 2018	11
FIGURE 5: SELECTED TOP MEDTECH MERGERS AND ACQUISITIONS WORLDWIDE IN 2017-2018, BY VALUE (IN BILLION US DOLLARS)	12
FIGURE 6: MAJOR MARKET SEGMENTATION 2018.....	13
FIGURE 7: NUMBER OF ALL HOSPITALS IN THE US FROM 1975 TO 2016.....	14
FIGURE 8: LEADING US MEDTECH REGIONS 2018.....	16
FIGURE 9: NORTH AMERICA'S DENTAL EQUIPMENT MARKET SIZE FROM 2012 TO 2020 BY PRODUCT (IN MILLION US DOLLARS).....	27
FIGURE 10: SHARE OF AMERICANS WHO UNDERWENT ORTHOPEDIC TREATMENT IN THE LAST 3 YEARS IN 2018, BY AGE.....	34
FIGURE 11: GLOBAL TOP 10 COMPANIES BASED ON ORTHOPEDIC MEDICAL TECHNOLOGY MARKET SHARE IN 2017 AND 2024.	35

List of Tables

TABLE 1: TRADE FLOWS OF MEDICAL DEVICES 2015	9
TABLE 2: TOP 10 MEDICAL DEVICE COMPANIES 2018.....	17
TABLE 3: KEY GROUP PURCHASING ORGANIZATIONS (GPOS)	19
TABLE 4: COMPANIES RANKED BY MEDICAL TECHNOLOGY R&D SPENDING WORLDWIDE IN 2017 AND 2024 (IN MILLION US DOLLARS).....	21
TABLE 5: US COMPANIES FOR CARDIOVASCULAR	22
TABLE 6: ASSOCIATIONS FOR CARDIOVASCULAR DISEASES	25
TABLE 7: US COMPANIES FOR DENTISTRY.....	28
TABLE 8: ASSOCIATIONS FOR DENTAL EQUIPMENT	30
TABLE 9: US COMPANIES FOR ONCOLOGY	31
TABLE 10: ASSOCIATIONS FOR ONCOLOGY	33
TABLE 11: US COMPANIES FOR ORTHOPEDICS	36
TABLE 12: ASSOCIATIONS FOR ORTHOPEDIC	38

1. General Market Overview

US Economy

The US economy has a highly developed and technologically-advanced service sector which generates 20% of the global output.¹ Table 1 demonstrates a general overview of US social and economic key figures.²

	Key Figures
Population	325.8 million US\$
Area in km ²	9.83 Mio. km ²
Capital	Washington D.C.
States	50 Federal States
Administrative Language	English Spanish (not an official administrative language)
Demographic Groups	76,6% White (18,1% Latino), 13,4% Afro-American, 5,8% Asian, 1,3% Natives (mainland), 0,2% Natives (island), 2,7% two or more ethnicities
GDP (nominal)	20.2 billion US\$
Share of GDP	Agriculture 0,9%, Industry 18,9%, Services 80,2%
Population Growth	0,71%
Unemployment Rate	3,9%
National Debt	20 billion US\$
Import	260.2 billion US\$
Import Partners	China 22,5%, Canada 12,9%, Mexico 12,7%, Japan 5,6%, Germany 4,8%
Export	213.8 billion US\$
Export Partners	Canada 18,1%, Mexico 17,4%, China 7,8%, Japan 4,5%, Germany 3,5%
Import Sectors (%)	Capital goods 26.7%, Consumer goods 26.2%, Industrial goods 22.6%, Motor vehicle industry 14.8%, Food & Beverages 5.7%, other 4%
Export Sectors (%)	Capital Goods 33.4%, Consumer Goods 13.4%, Industrial Goods 31%, Automotive Industry 10.4%, Food & Beverage 8%, other 3.5%

¹ Source: Focus Economics (2018), [United States Economy Overview](#), retrieved on 13.12.2018

² Source: United States Census Bureau (2018): [Quick Facts United States](#) und [U.S International Trade in Goods and Services](#), retrieved on 13.12.2018

1.1. An Introduction to the US medical technology industry

The medical technology industry is a vital part of the healthcare sector and is a very competitive landscape. The global market size of the medtech industry generates an estimate of 430 billion US\$ annually, with established centers in the United States (US) and Europe. Trends, however, show that China is to become a more prominent player in the coming years.³

The United States remains a driving force in the medtech industry with the largest market in the world. The US industry for medical device manufacturing in 2018 generated a revenue of 39.5 billion US\$ with a profit of 1.8 billion US\$.⁴ It is home to primary division leaders such as Johnson & Johnson Medical Devices & Diagnostics and General Electric Health.⁵ The expected annual growth from 2018 to 2023 is 3.0%.

Even though the US is experiencing strong domestic growth, the expected revenue of 11.9 billion US\$ made in exports, is projected to fall annually by less than (>) 2%. With China on the rise and continued globalization, the industry will experience a shift in the next five years. International companies will increasingly outsource manufacturing and research and development, thus reducing the number in domestic operators.⁶

Through market capitalization and sector rotation, bigger tech companies are expanding into the industry of health services. Medtech market capitalization outpaced the broader markets of the healthcare sector. Hence, the medTech industry is undergoing a transition, adapting to fundamental shifts in reimbursement, consumer empowerment and digital enablement.⁷

The companies are globally respected for their innovative and advanced technology.⁸ 80% of American medical device companies are small and medium enterprises and consist of fewer than 50 employees. Overall, the US medtech industry sector employs over 2 million people. According to the 2016 Top Markets Report on Medical Devices, the US exported 43.2 billion US\$ and imported an estimate of 49.9 billion US\$ in medical devices.⁹

The top companies of the medical device industry are located in the US and generate the highest revenue worldwide. US companies produce up to 50 % more revenue than that of their European competitors. In 2017 the US medtech industry made

³ Source: Statista (2018) [Medical technology industry](#), retrieved on 03.01.2019

⁴ Source: Statista (2018), [Leading U.S. medtech regions](#), retrieved on 12.12.2018

⁵ Source: Statista (2018) [Medical technology industry](#), retrieved on 03.01.2019

⁶ Source: IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019


⁷ Source: EY (2016), [Pulse of the Industry](#), retrieved on 13.12.2018

⁸ Source: International Trade Administration (2016), [2016 Top Markets Report Medical Device](#), retrieved on 07.01.2018

⁹ Source: International Trade Administration (2016) [2016 Top Markets Report Medical Devices](#), retrieved on 07.01.2019

225.1 billion US\$ in revenue. Figure 1 shows the total revenue of US and European medical technology companies from 2009 to 2017 in billion US\$. Both markets combined generated a revenue of 379.1 billion US\$ in 2017.

Figure 1: Total revenues of US and European medical technology companies

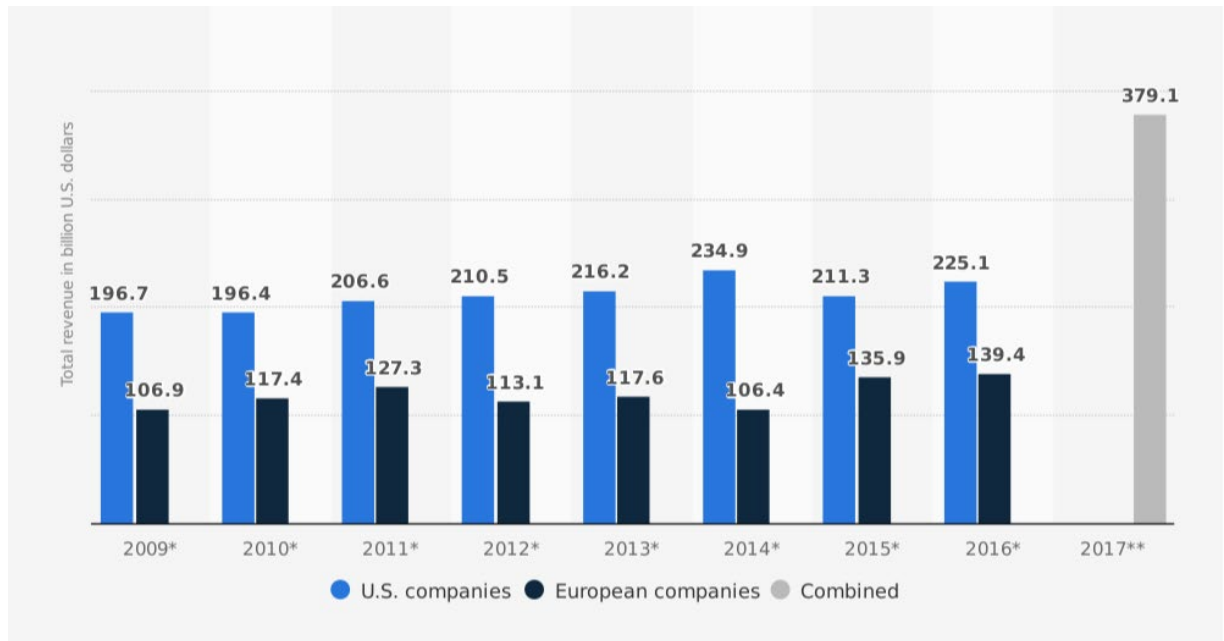

Source: Statista (2018) [Total revenue of US and European medical technology companies from 2009 to 2017 \(in billion US\\$\)](#), retrieved on 15.04.2019

1.1.1. Export and Import of Medical Devices

Traditionally, the medical device manufacturing industry is known for in-house sourcing. Shifts in the medtech industry are driving experienced companies to outsource to niche companies though. Stronger profit margins allow for general tech companies to invest in facility infrastructure and specialize in equipment to manufacture their own medical devices.

With a globalizing world, the trend for many companies is to move production to other countries as to minimize transaction cost. Moreover, in place of exporting, medical devices that are produced outside the US are manufactured to comply with regulations and quality controls of that country. Even though, the regulatory framework of medical devices is being more and more coordinated under the direction of the World Health Organization to allow easier access to different national markets and uphold standards, each country applies an altered framework.

As illustrated in Table 2, manufacturers in the medical technology industry operate in the area of in-vitro diagnostic substance, electro-medical apparatus, irradiation apparatus, surgical and medical instruments, surgical appliances and supplies, dental equipment and supplies and ophthalmic goods.

Table 1: Trade flows of Medical Devices 2015

Sectors	2015 Exports (Billion US\$)	2015 Imports (Billion US\$)
In Vitro Diagnostic Substance	6.1	3.5
Electro-medical Apparatus	7.5	10.3
Irradation Apparatus	3.6	3.7
Surgical and Medical Instruments	12.4	12.3
Surgical Appliances and Supplies	9.6	13.7
Dental Equipment and Supplies	1.2	1.3
Ophthalmic Goods	2.7	5.1
Total	43.2	49.9

In 2017 the US export of medical devices exceeded 41 billion US\$ in key product categories.¹⁰ The result of emerging markets is a decrease in exports at an annual rate of 2% valued at 11.9 billion US\$ and an increase of imports at an annual rate of 4.0% with 17.3 billion US\$ over a five year span to 2018.

Because many manufacturers are establishing operations abroad, countries no longer need to import devices from the US. Emerging markets such as China and Singapore made significant progress and are investing in their own medical device manufacturing industry. 3D bio-printing is a technology that is especially on the forefront of product development and receives significant attention from Asian countries, thus decreasing dependence on the US for scientific research.

Figure 2 and 3 highlight China as one of the strongest trade partners to the US for medical devices. Yet the highest importing country to serve the US market is Germany which further receives in return 9.5% of the exports from the US.¹¹

¹⁰ Source.: International Trade Administration (2016), [2016 Top Markets Report Medical Device](#), retrieved on 07.01.2018

¹¹ IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

Figure 2: Imports


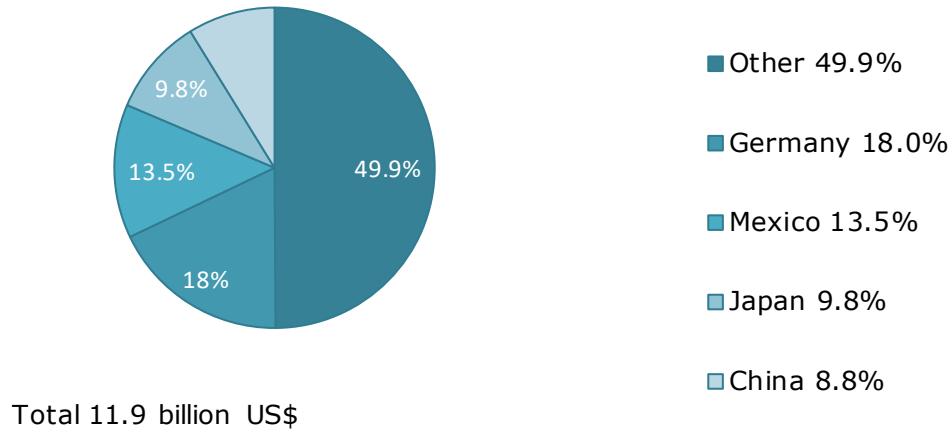


Figure 3: Exports

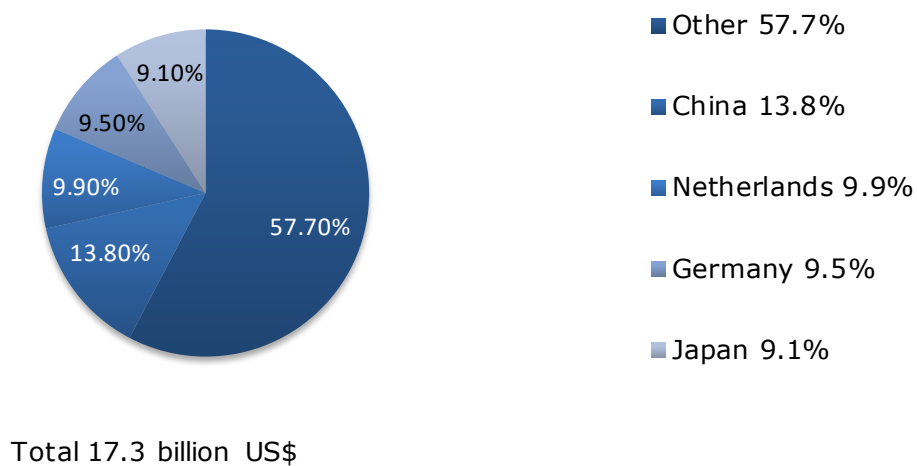


The medical device industry is a highly competitive market with various small innovative niches. Many companies have a similar product line and overlap in specific

sectors. With the market being saturated, bigger companies use their advantage to sell a product at a better bargain price to hospitals and other end-consumers.¹²

Even though small and medium sized companies do not necessarily have the monetary reserves comparable to their larger competitors, their focus on niche markets provides them with an advantage to produce specialized medical devices and thus can incorporate bigger corporations as a buyer. This approach allows the number of operators in the industry to grow annually over the next five years at an estimated rate of 1.9% to 927 operators by 2023, consequently pushing industry employment at an annually rate of 2.4% to 94,864 individuals.

The products and service segmentation in Figure 4, presents the estimated industry revenue of the sectors for diabetes devices, cardiovascular devices, irradiation devices, patient recovery and noninvasive devices and others, that together form a total revenue of 39.5 billion US\$.

Figure 4: Products and service segmentation 2018

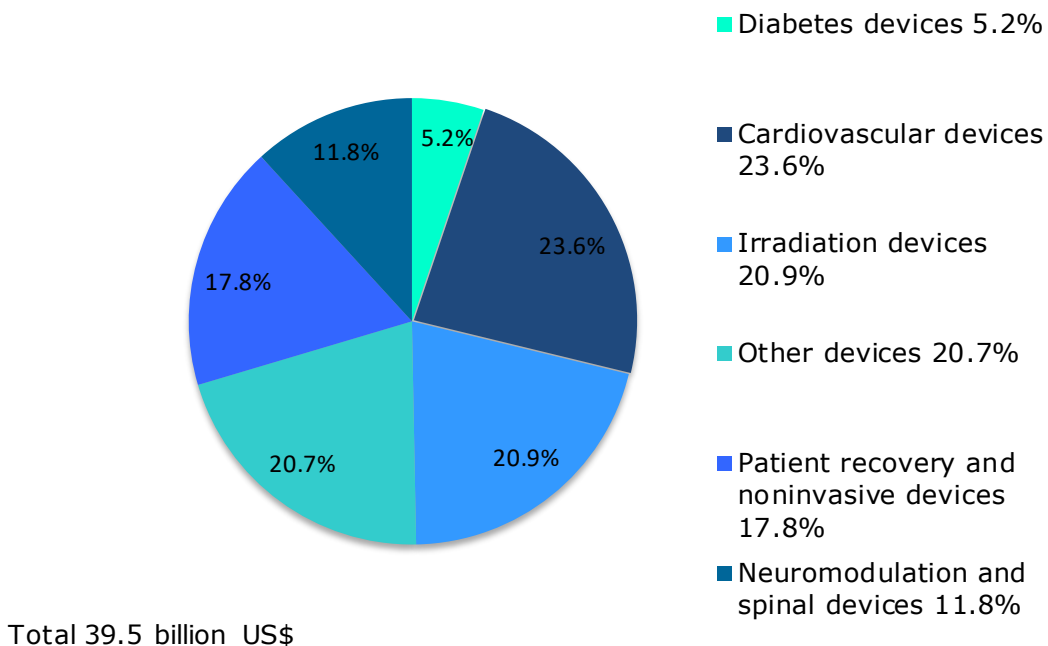

Source: IBISWorld¹³

¹² Source: IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019


¹³ Source: IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

Digital MedtTech is one of the new emerging trends according to an executive of a MedTech association. It has a broad proposition covering multiple areas of innovation all characterized by new and evolving ways to generate, parse, and leverage data. Wearable and implantable diagnostics, potentially combined with therapeutic interventions that likely will be increasingly AI-driven, for example, hold great promise to continue to improve care. Diagnostics continues to play an increasingly important role in patient care. The surface in terms of precisions diagnostics, calibrating drug regimens for example to maximize their effectiveness for individuals, has only begun to be touched upon.¹⁴

1.1.2. Economies of scale

Important elements that influence the success of medtech companies are the size of the companies, access to new technology, access to a highly skilled workforce and contacts within key markets. Particularly companies with large manufacturing facilities are able to reduce costs and selling prices while maintaining profit margins. Through large mergers and acquisitions the big medtech companies are able to consolidate their strong position in the medical technology industry.¹⁵

Figure 5: Selected top medtech mergers and acquisitions worldwide in 2017-2018, by value (in billion US dollars)

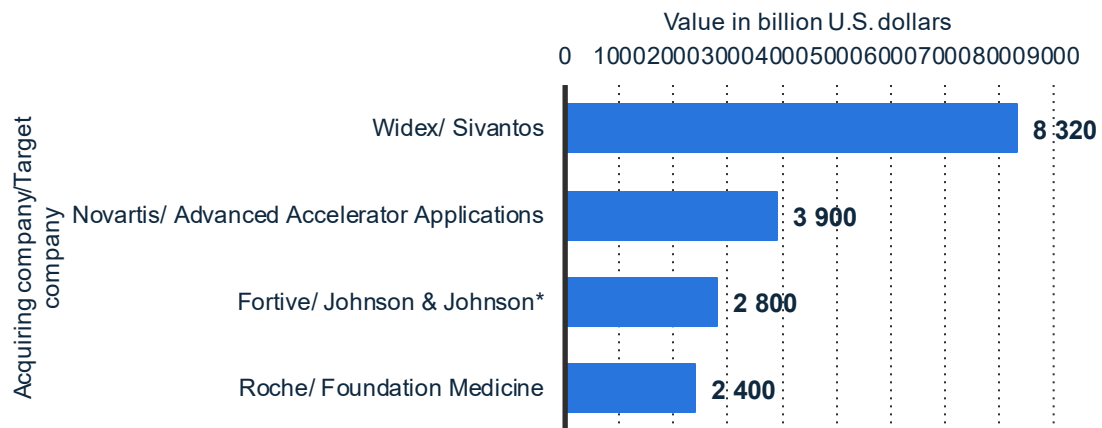

Source: Statista (2018) [Medical technology industry](#), retrieved on 17.01.2019

The biggest mergers between 2017 and 2018, as shown in Figure 5, were between Widex and Sivantos with a value 8.320 billion US\$, Novartis and Advanced Accelerator Applications with a value of 3.900 billion US\$ and the merger of Fortive and Johnson & Johnson with a value of 2.800 billion US\$

¹⁴ Interview with an Associate of a Medical Technology Association from 10.01.2019


¹⁵ Source: IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

1.1.3. Markets for Medical Technology

The major market for medical devices are hospitals, which account for a 35.9% share of the market. Hospitals tend to be near densely populated areas, which allow easier access for patients, as the number of physician's visits are in direct correlation with the demand for medical devices. In general, medical and surgical hospitals predominantly require specific machinery for different therapeutic areas and tend to purchase machinery and products in greater quantities. Smaller, community-based hospitals on the other hand, have slightly different needs and require various types of electro-medical and electrotherapeutic products.¹⁶

Distributors account for 25.2% of the medical device market and are seen as the link between medical device manufacturers and healthcare providers. Distributors are wholesalers that purchase large amounts of medical and surgical equipment from manufacturers and redistribute.¹⁷

Figure 6: Major market segmentation 2018

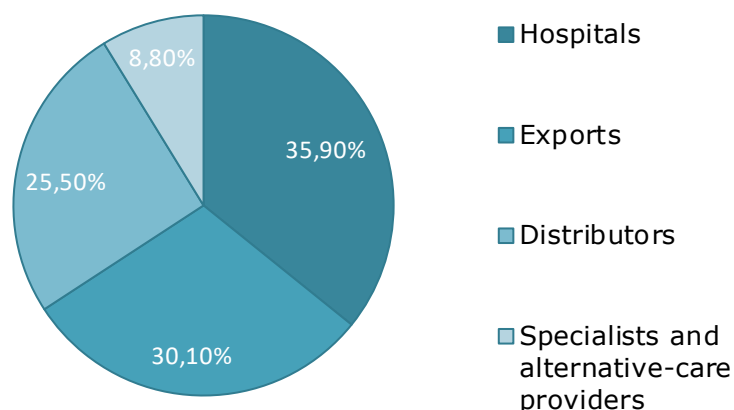

Total 39.5 billion US\$


Group purchasing organizations (GPOs) are groups of businesses that are able to bargain with vendors based on their collective buying power. Especially in the health-care sector, GPOs maintain a close relationship with key distributors. The main markets for medical device manufacturers are hospitals, clinics, specialists and alternate-care providers. Long-term contracts are conducted with vendors that are able to sell on a group price.

¹⁶ Source: IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

¹⁷ Source: IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

Figure 7 illustrates the total number of hospitals in the US from 1975 to 2016. The number of hospitals in the US has shown a steady decline. Since 2000, the number fell from over 5,800 to less than 5,600 facilities. Yet, due to US healthcare expenditures, hospitals remain one of the largest markets for the health and medical device manufacturer sector.

Figure 7: Number of all hospitals in the US from 1975 to 2016

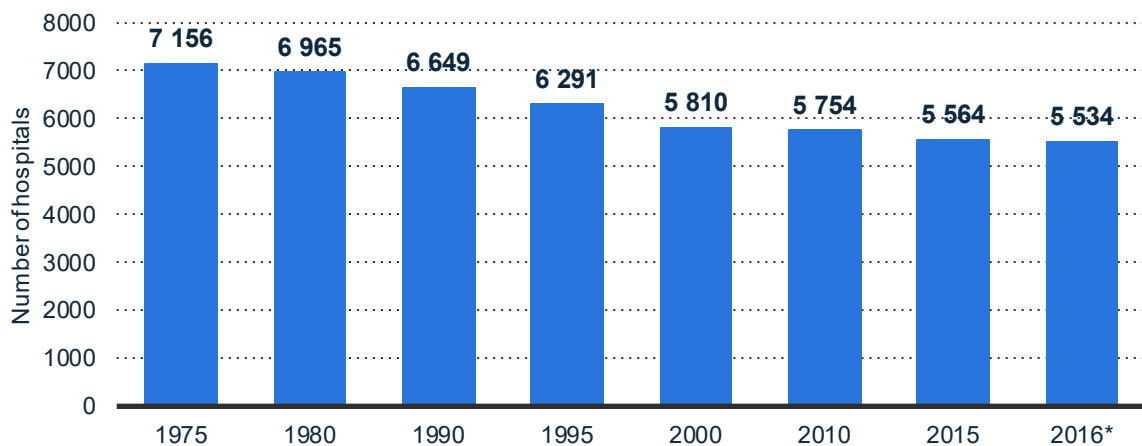

Source: Statista (2018), [Number of all hospitals in the U.S. from 1975 to 2016](#), retrieved on 16.01.2019

According to another specialist of a MedTech association, the fundamentals continue to be strong. There are boundless opportunities to continue to save and improve lives. The factors such as a worldwide aging population, expanding middle classes in emerging economies that are increasingly seeking the best available care, and the continued need for solutions for the world's healthcare challenges are considered a good foundation for continued growth.¹⁸

1.1.4. External Drivers

Number of physician visits

One of the largest groups of medical device buyers are hospitals. The number of purchases correlates to the number of physician visits in a year and government funding. An increase in physician visits will positively affect the demand for medical devices.¹⁹

Number of adults aged 65 and older

With an aging population and longer life expectancy, the incidences of diseases and disorders are on a rise. In view of that, the need for early on recognition and medical

¹⁸ Interview with an Associate of a Medical Technology Association from 10.01.2019

¹⁹ Source: IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

treatment becomes indispensable. The number of adults aged 65 and older is expected to increase in the coming years.²⁰

Total health expenditure

The total health expenditure concerns private and public spending. Healthcare funding programs are intended to enable greater funding for the replacement of medical equipment and supplies. This should allow for an increase in industry demand.²¹

Federal funding for Medicare and Medicaid

More and more people are getting access to Medicare, significantly affecting physician visits and access to treatments which is considered a positive development. Health coverage is a vital factor in the US. Medicare coverage allows patients to invest in medical devices, that otherwise would not be affordable. Federal funding for Medicare and Medicaid is expected to increase.²²

Trade-weighted Index

The trade-weighted Index is an important factor concerning the purchase of medical devices. A high trade-weighted index suppresses the purchase of domestically manufactured devices due to higher costs in purchasing. For that reason, the strong dollar poses a threat to the industry.²³

1.1.5. Economic Growth of Medical Technology by Region

The medical technology industry is clustered across the US. Thus, different states are important to different sectors of the industry. The largest medtech hubs are found in California for medical device manufacturing and Massachusetts for its cutting edge research centers. New York and New Jersey have major academic medical institutions. As shown in Figure 8, the command centers of the world's top tech companies are located in California, Massachusetts, New York and New Jersey.


²⁰ Source: IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

²¹ Source: IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

²² Source: IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

²³ Source: IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

Figure 8: Leading US medtech regions 2018

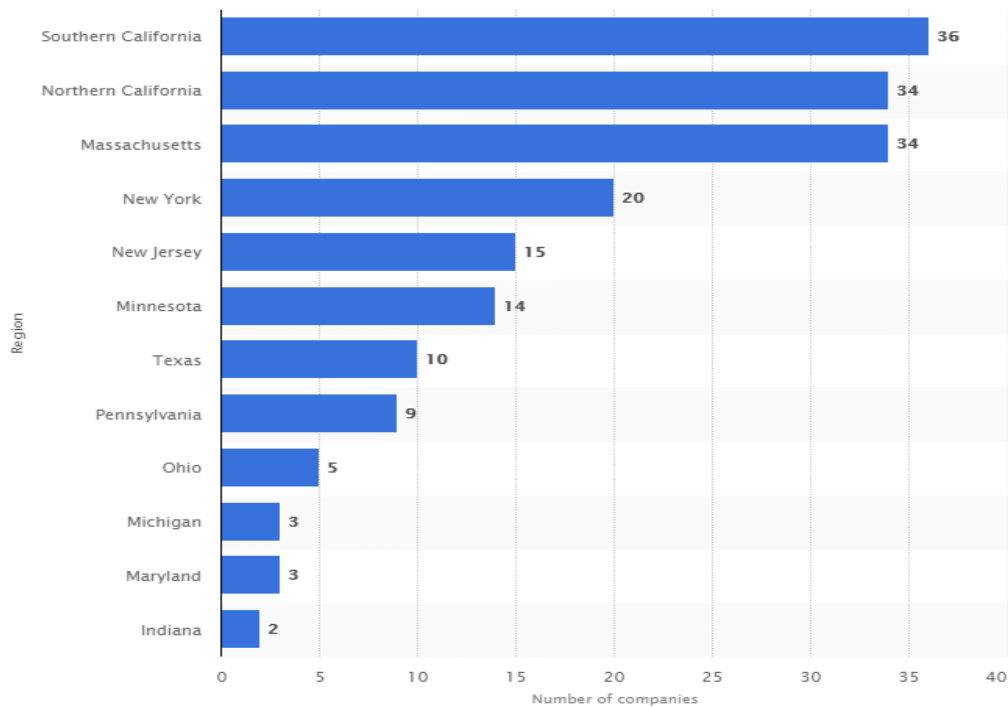

Source: Statista (2018) [Medical Technology Industry](#), retrieved on 16.01.2019

According to Winthrop Turlow, the Executive Director of the MedTech Association, more and more companies are settling in the states around the Great Lakes, due to lower costs in production and rates in taxation. As many other small and medium sized businesses tend to settle around the Great Lakes, new smaller specialized medtech hubs are established.²⁴

The distribution of medtech establishments and other high-technology industries is driven by various key factors. Thus geographic distribution, proximity to complementary industries, location of customers, suppliers, and high-skilled labor are considered important factors.²⁵

²⁴ Interview with Winthrop Turlow, Executive Director of MedTech Association from 10.01.2019

²⁵ Source: IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

1.1.6. Medical Device Companies and Key distributors

Table 2 shows the top 10 global Medical Device companies based on the revenue they generated in 2018. The three leading companies in 2018 are Medtronic, DePuy Synthes and Fresenius. Overall seven of the ten medical device companies are located in the US.

Table 2: Top 10 Medical Device Companies 2018

Company	Revenue
1 – Medtronic, US	29.95 billion US\$
2 – DePuy Synthes, Johnson & Johnson, US	26.6 billion US\$
3 – Fresenius, DE	20.7 billion US\$
4 – Philips Healthcare, NL	20.7 billion US\$
5 – GE Healthcare, US	19.1 billion US\$
6 – Siemens Healthineers, DE	16.5 billion US\$
7 – Cardinal Health, US	13.5 billion US\$
8 – Stryker, US	12.4 billion US\$
9 – Becton Dickinson, US	12.1 billion US\$
10 – Baxter, US	10.6 billion US\$

1.1.7. Profile of the top three US medical technology companies

Medtronic (HQ Minneapolis, Minnesota)

Medtronic is an US-Irish medical technology company. After a 48 billion US\$ merger with Covidien in 2015, Medtronic positioned itself as the dominant market leader for cardiovascular technology, services and solutions. Owning 22.6% of the market, their leading revenue segment encompasses the Cardiac and Vascular Group, followed by Minimally Invasive Therapies, Restorative Therapies, and the Diabetes Group.²⁶ Below is a comprised list of the sectors Medtronic services and what devices are in their product line. The revenue is based on their fiscal year in 2018.

²⁶ Source: Statista (2018), [Distribution of Medtronic's revenue from 2014 to 2018, by segment \(in million U.S. dollars\)](#), retrieved 14.01.2019

Sector	Devices	2018
Cardiac and Vascular	Aortic and Peripheral Vascular Cardiac Rhythm and Heart Failure Coronary and Structural Heart	11.4 billion US\$
Minimally Invasive Therapies	Renal Care Solutions Respiratory, Gastrointestinal, and Informatics Surgical Innovations	8.7 billion US\$
Restorative Therapies	Spine Brain Therapies Pain Therapies Specialty Therapies	7.7 billion US\$
Diabetes	Advanced Insulin Management Multiple Daily Injection Solutions Non-Intensive Diabetes Therapies	2.1 billion US\$

DePuy Synthes /Johnson & Johnson (HQ Warsaw, Indiana)

Johnson & Johnson's subsidiary company DePuy Synthes produces an array of medical devices and comes in second, after Medtronic, with 27 billion US\$ in revenue.²⁷ They cover the sectors of orthopedic, cardiovascular, diabetes, vision care and surgery. Best selling products are in the fields of surgical vision, wound closure, bio-surgery, and electrophysiology.²⁸ Below is a comprised list of the sectors DePuy Synthes services and the devices they manufacture. The revenue is based on their fiscal year of 2018.²⁹

Sector	Devices	2018
Diabetes	Diabetes Care Diagnostics Interventional Solutions	1 millions US\$
Orthopedics	Hips Knees Trauma Spine & other	8.9 millions US\$
Surgery	Advanced General Specialty	9.9 millions US\$
Vision	Contact Lenses Surgical	4.6 millions US\$

²⁷ Source: Hoovers (2018), [Depuy Synthes, Inc.](#), retrieved on 22.01.2019

²⁸ Source: IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

²⁹ Source: Johnson & Johnson (2018), [Reported Sales vs Prior Period \(\\$MM\)](#), retrieved on 22.01.2019

Total Medical Devices	27 millions US\$
------------------------------	------------------

General Electric Healthcare (HQ Milwaukee, Wisconsin)

GE Healthcare, headquartered in US in Fairfield, Connecticut, attributes its growth to emerging markets of South East Asia and Latin America. With a revenue of 18 billion US\$ in 2017, their focus areas are 'Healthcare Systems' and imaging products, particularly mammography and CTS (computerized tomography).³⁰ Their areas of specialties comprise oncology, cardiology, and stroke. The revenue is based on their fiscal year in 2017.³¹

Sector	Devices	2017
Diagnostic imaging & services	Magnetic resonance Computed tomography Molecular imaging X-ray systems	8 billion US\$
Mobile diagnostic & monitoring	Ultrasound Clinical Solutions Monitoring Mobile Health	4 billion US\$
IT & digital Solutions	Enterprise Imaging Financial Management Care Area Workflows GE Health Cloud TM	2 billion US\$
Life Sciences	Bio process Protein & Cell Sciences Contrast Media & Nuclear Tracers Cellular Therapy	4 billion US\$

1.1.8. Key Distributors (Group Purchasing Organizations)

Table 3 shows the top GPOs in the US. GPOs maintain direct contact with hospitals, caregivers, and third-party service providers that require medical instruments. They strongly depend on their relationship with medtech companies and other vendors to serve their clients in the healthcare sector.

Table 3: Key Group Purchasing Organizations (GPOs)

³⁰ Source: IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

³¹ Source: GE (2018), [GE Healthcare](#), retrieved on 22.01.2019

Company	Revenue
1- <u>AmerisourceBergen</u>	153 billion US\$
2- <u>Cardinal Health</u>	136 billion US\$
3- <u>HealthTrust Purchasing Group</u>	64 million US\$
4- <u>Henry Schein</u>	12 billion US\$
5- <u>Intalere</u>	44 million US\$
6- <u>McKesson Pharmaceutical</u>	5.2 million US\$
7- <u>Premier Inc</u>	1.6 billion US\$
8- <u>Provista</u>	5.8 million US\$
9- <u>Vizient</u>	1 billion US\$
10 - MedAssets (Vizient)	529 million US\$

1.1.9. Research and Development

The United States leads in the Research and Development of the medical technology industry. Expenditures for Research and Development (R&D) average a 7% of revenue. The medical device industry and many government institutions invest in R&D. A peak of R&D spending was reached in 2016 with an investment of 12.8 billion US\$. The biggest spenders on R&D were Medtronic and Abbot Laboratories as shown in Table 4. It is expected that larger medtech companies will expand their R&D budget plan by approximately 3% by the year of 2020.

Table 4: Companies ranked by medical technology R&D spending worldwide in 2017 and 2024 (in million US dollars) ³²

Company	2017	2024
Medtronic (US)	2.253	2.738
Abbot Laboratories (US)	1.640	2.351
Philips (NL)	1.728	2.204
Johnson & Johnson (US)	1.610	2.024
Siemens (DE)	1.416	1.760
Roche (CH)	1.378	1.411
Boston Scientific (US)	974	1.381
Becton Dickinson (US)	774	1.365
Danaher (US)	939	1.293
Stryker (US)	787	1.152

The table above comprises the top 10 technology companies with the highest projected spending in 2024. The strongest European players are Philips followed by Siemens. US companies, nonetheless, remain the largest group of investors in the R&D medtech industry.

Research and development is a key element of health sciences. It defines the parameters and allows for future growth. With digital technology on the rise, and merging market sectors, international companies invest in acquiring small, innovative companies instead of in-house R&D. As in the opinion of Winthrop Turlows, it becomes easier and more cost effective to outsource operations and establish collaborations, rather than to cultivate new sectors.³³

³² Source: Statista (2017), [Top 20 companies based on medical technology R&D spending worldwide in 2017 and 2014 \(in million U.S. dollars\)](#), retrieved on 09.01.2019

³³ Interview with Winthrop Turlow, Executive Director of MedTech Association from 10.01.2019

1.2. Cardiovascular

1.2.1. Medical Technological Market for Cardiovascular Diseases

With cardiovascular disease (CVD) being the leading cause of death for men and women in the US, cardiology represents one of the largest sectors of the medtech industry in the US. According to the American Heart Association (AHA), 82.6 million people in the United States are affected by one or more forms of cardiovascular disease.³⁴ With the rising number of people being affected through diabetes, obesity, poor diet, and lack of physical activity, the cardiovascular sector is expected to grow annually.

1.2.1.1. Market Size & Growth

The cardiologist industry produced a revenue of 30 billion US\$ and net earnings of 3.1 billion US\$ in 2018 and is expected to grow at 5.7% by 2022 with an estimated sales volume of 62.3 billion US\$.³⁵ The industry is in high demand for operators and currently provides employment to 86.000 employees.³⁶

1.2.1.2. US companies for Cardiovascular³⁷

The table below displays the biggest cardiovascular companies in the US market in alphabetical order.

Table 5: US companies for Cardiovascular

Companies	Key figures
Abiomed ³⁸	
Headquarters	Danvers, Massachusetts
Employees	1.100
Corporate Family	8 companies
Annual Sales	593 billion US\$
Total Assets	887 million US\$

³⁴ Source: National Academies Press (US), [A Nationwide Framework for Surveillance of Cardiovascular and Chronic Lung Diseases](#), retrieved on 18.01.2019

³⁵ Source: Medtronic (2018), [Facts and Statistics](#), retrieved on 14.01.2019

³⁶ Source: IBISWorld (2017), [Cardiologists Industry in the US](#), retrieved on 14.01.2019

³⁷ Source: Statista (2017), [Global top 10 companies based on cardiologic medical technology market share in 2017 and 2024](#), retrieved on 09.01.2019

³⁸ Source: Hoovers (2018), [Abiomed](#), retrieved on 18.01.2019

Abbott Laboratories ³⁹ Headquarters Employees Corporate Family Annual Sales Total Assets	North Chicago, Illinois 99.000 768 companies 27 billion US\$ 71 billion US\$
Boston Scientific ⁴⁰ Headquarters Employees Corporate Family Annual Sales Total Assets	Marlborough, Massachusetts 29.000 266 companies 9 billion US\$ 20 billion US\$
Edwards Lifesciences ⁴¹ Headquarters Employees Corporate Family Annual Sales Total Assets	Irvine, California 12.000 51 companies 3.4 billion US\$ 5.9 billion US\$
Getinge ⁴² Headquarters Employees Corporate Family Annual Sales Total Assets	Wayne, New Jersey 600 214 186 million US\$ 90 million US\$
Johnson & Johnson ⁴³ Headquarters Employees Corporate Family	New Brunswick, New Jersey 134.000 910 companies

³⁹ Source: Hoovers (2018), [Abbott Laboratories](#), retrieved on 18.01.2019

⁴⁰ Source: Hoovers (2018), [Boston Scientific](#), retrieved on 18.01.2019

⁴¹ Source: Hoovers (2018), [Edwards Lifesciences](#), retrieved on 18.01.2019

⁴² Source: Hoovers (2018), [Getinge](#), retrieved on 18.01.2019

⁴³ Source: Hoovers (2018), [Johnson & Johnson](#), retrieved on 18.01.2019

Annual Sales Total Assets	76 billion US\$ 155 billion US\$
Medtronic ⁴⁴ Headquarters Employees Corporate Family Annual Sales Total Assets	Minneapolis, Minnesota 49.000 609 companies 19 billion US\$ 55 billion US\$
Terumo ⁴⁵ Headquarters Employees Corporate Family Annual Sales Total Assets	Somerset, New Jersey 3.4.000 177 companies 758 million US\$ 288 million US\$
W.L. Gore & Associates ⁴⁶ Headquarters Employees Corporate Family Annual Sales Total Assets	Newark, Delaware 9.800 78 companies 3.4 billion US\$ N/A

⁴⁴ Source: Hoovers (2018), [Medtronic](#), retrieved on 18.01.2019

⁴⁵ Source: Hoovers (2018), [Terumo](#), retrieved on 18.01.2019

⁴⁶ Source: Hoovers (2018), [W.L. Gore & Associates](#), retrieved on 18.01.2019

1.2.2. Associations for cardiovascular diseases

Shown in the table down below are prominent associations working in the field of cardiovascular disease.

Table 6: Associations for cardiovascular diseases

Associations	Links
American Heart Association	<u>AHA</u>
American College of Cardiology	<u>ACC</u>
Heart Rhythm Society	<u>HRS</u>
National Heart Foundation	<u>NHF</u>
World Heart Federation	<u>WHF</u>
US Department of Health and Human Services	<u>HHS</u>

1.3. Dentistry

1.3.1. Medical Technological Market for Dentistry

The US dental market is the largest globally. A special focus, due to Medicare, is being placed on oral health and greater insurance schemes that are more advantageous for potential patients. There is a rising demand for dental procedures in the field of restorative and surgical procedures. Those procedures are likely to create growth in the dental equipment market.⁴⁷

1.3.1.1. Market Size & Growth

The total value of the dental equipment industry over the past five years has grown by 2.5% and is expected to produce a revenue of 135 billion US\$ by 2019.⁴⁸ Due to the growing economic restoration and investment into healthcare the number of businesses has grown by 0.7% to 185,601. Due to aging population, an increased demand for cosmetic dentistry and an growing incidence of tooth decay, the market for dental equipment is expected to experience an annual growth of 2.1% to 131.7 billion US\$.⁴⁹

Over the past five years, the Dental Equipment Dealers industry has grown by 2.4% to reach revenue of 13 billion US\$ in 2018. In the same timeframe, the number of businesses has grown by 1.5% and the number of employees has grown by 1.8%.


Figure 9 shows the expected growth of dental equipment in the fields of dental laser, hygiene maintenance devices, laboratory machine, dental radiology equipment, systems and parts, and other equipment by 2020.

⁴⁷ Source: IBISWorld (2018), [Dental Equipment Dealers Industry in the US](#), retrieved on 14.01.2019

⁴⁸ Source: IBISWorld (2018), [Dental Equipment Dealers Industry in the US](#), retrieved on 14.01.2019

⁴⁹ Source: IBISWorld (2018), [Dental Equipment Dealers Industry in the US](#), retrieved on 14.01.2019

Figure 9: North America's dental equipment market size from 2012 to 2020 by product (in million US dollars)⁵⁰

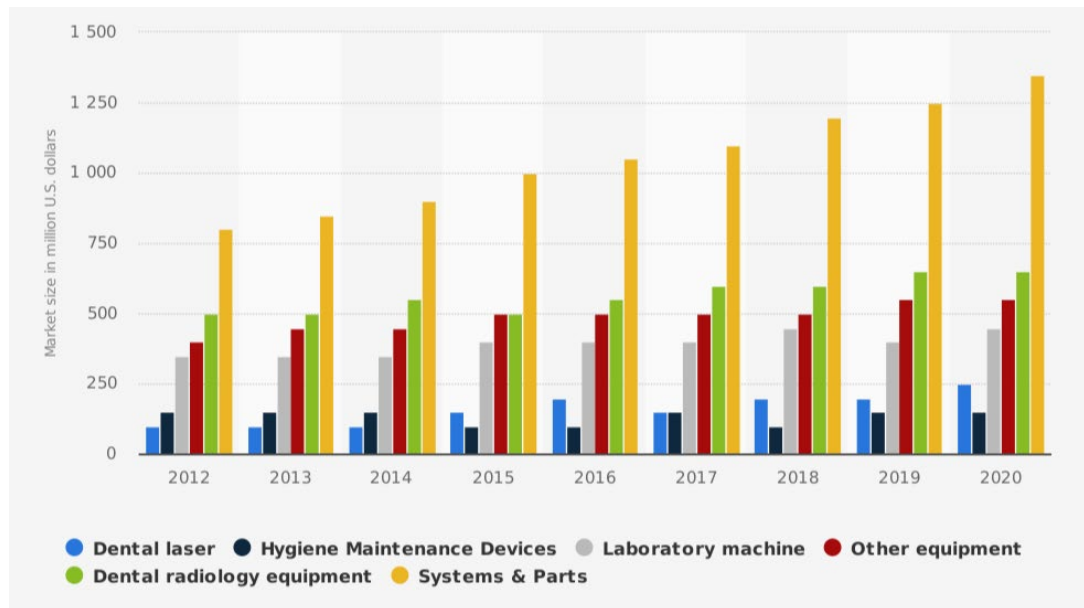

The service sector of dentistry in the US consists of dental consultation and diagnostic services, preventative services, restorative dental services, prosthodontics, orthodontics, surgical oral and maxillofacial services and nonsurgical endodontic services.

⁵⁰ Source: Statista (2016) , [North America's dental equipment market size from 2012 to 2020, by product \(in million U.S. dollars\)](#), retrieved on 17.01.2019

1.3.1.2. US companies for Dentistry

The table down below displays the major dentistry equipment manufacturers in the US market in an alphabetical order.

Table 7: US companies for Dentistry

Companies	Key figures
A-dec Inc. ⁵¹ Headquarters Employees Corporate Family Annual Sales Total Assets	Newberg, Oregon 1.900 4 companies 310 million US\$ 19 million US\$
AMD Lasers ⁵² Headquarters Employees Corporate Family Annual Sales Total Assets	Indianapolis, Indiana 16 N/A 2.6 million US\$ N/A
Biolase, Inc. ⁵³ Headquarters Employees Corporate Family Annual Sales Total Assets	Irvine, California 195 3 companies 46 million US\$ 34 million US\$
Carestream Health ⁵⁴ Headquarters Employees Corporate Family Annual Sales Total Assets	Rochester, New York 7.000 982 companies 2 billion US\$ N/A

⁵¹ Source: Hoovers (2019), [A-dec](#), retrieved on 14.01.2019

⁵² Source: Hoovers (2019), [AMD Lasers](#), retrieved on 14.01.2019

⁵³ Source: Hoovers (2019), [Biolase](#), retrieved on 14.01.2019

⁵⁴ Source: Hoovers (2019), [Carestream Health](#), retrieved on 14.01.2019

Danaher Corporation ⁵⁵ Headquarters Employees Corporate Family Annual Sales Total Assets	Washington, DC 67.000 646 companies 18 billion US\$ 47 billion US\$
Dentsply Sirona ⁵⁶ Headquarters Employees Corporate Family Annual Sales Total Assets	York, Pennsylvania 16.000 95 companies 3.9 billion US\$ 8.7 billion US\$
Henry Schein ⁵⁷ Headquarters Employees Corporate Family Annual Sales Total Assets	Melville, New York 700 354 Companies 12 billion US\$ 7.8 billion US\$
3M ⁵⁸ Headquarters Employees Corporate Family Annual Sales Total Assets	Saint Paul, Minnesota 91.000 656 companies 31 billion US\$ 37 billion US\$
Patterson Companies, Inc. ⁵⁹ Headquarters Employees Corporate Family Annual Sales Total Assets	Saint Paul, Minnesota 7.700 207 companies 5.4 billion US\$ 1.2 billion US\$

⁵⁵ Source: Hoovers (2019), [Danaher Corporation](#), retrieved on 23.01.2019

⁵⁶ Source: Hoovers (2019), [Dentsply Sirona](#), retrieved on 14.01.2019

⁵⁷ Source: Hoovers (2019), [Henry Schein](#), retrieved on 23.01.2019

⁵⁸ Source: Hoovers (2019), [3M](#), retrieved on 14.01.2019

⁵⁹ Source: Hoovers (2019), [Patterson Companies, Inc.](#), retrieved on 14.01.2019

1.3.2. Associations for dental equipment

Shown in the table down below are prominent associations for dentistry.

Table 8: Associations for dental equipment

Associations	Links
American Dental Association	ADA
American Board of Pediatric Dentistry	ABPD
American Dental Education Association	ADEA
America's Pediatric Dentists	APD
Dental Trade Alliance	DTA

1.4. Oncology

1.4.1. Medical Technological Market for Oncology

The market for oncology is divided into segments and encompasses diagnosis and treating of cancer diseases with medical devices, in-vitro diagnostics and combination device products.⁶⁰ Early detection is vital. With the trend of big data mapping and new modalities in technological advancements, the market is expanding. Connectivity and internet-related devices, allow for better tracking. Endoscopic devices are projected to account for a major share because of the growing preference for these devices.⁶¹ Screening of the infected site helps in early cancer detection. Especially the field of pharmaceuticals and research on cancer has been pushing the market growth of oncology in health sciences.⁶²

It is estimated that 1.735.350 new cases of cancer would be diagnosed in 2018.⁶³ The most common cancer according to the National Cancer Institute are breast cancer, lung and bronchus cancer, prostate cancer, colon and rectum cancer, melanoma of the skin, bladder cancer, non-Hodgkin lymphoma, kidney and

⁶⁰ Source: FDA (2018), [Oncology Devices and Diagnostics](#), retrieved on 18.01.2019

⁶¹ Source: Statista (2018), [Oncology](#), retrieved on 17.12.2018

⁶² Source: Wiley Online Library (2018), [Cancer Statistics 2018](#), retrieved on 23.01.2019

⁶³ Source: Transparency Market Research (2018), [Oncology Devices Market](#), retrieved on 15.01.2019

renal pelvis cancer, endometrial cancer, leukemia, pancreatic cancer, thyroid cancer, and liver cancer.⁶⁴

1.4.1.1. Market Size & Growth

National expenditures for cancer care in the United States in 2017 averaged at 147.3 billion US\$. Costs are likely to rise in the coming years as the population ages and cancer prevalence increases. Moreover, costs are likely to rise as new, and often more expensive, treatments are adopted as standard of care.⁶⁵

1.4.1.2. US companies for Oncology

The table below displays the major oncology equipment manufacturers in the US market in alphabetical order.

Table 9: US companies for Oncology

Companies	Key figures
Accuray ⁶⁶ Headquarters Employees Corporate Family Annual Sales Total Assets	Sunnyvale, California 959 15 companies 404 million US\$ 369 million US\$
Allogene Therapeutics ⁶⁷ Headquarters Employees Corporate Family Annual Sales Total Assets	South San Francisco, California 78 N/A 1.7 million US\$ 148 million US\$

⁶⁴ Source: National Cancer Institute (2018), [Cancer State](#), retrieved on 18.01.2019

⁶⁵ Source: National Cancer Institute (2018), [Cancer State](#), retrieved on 18.01.2019

⁶⁶ Source: Hoovers (2019), [A-dec](#), retrieved on 14.01.2019

⁶⁷ Source: Hoovers (2019), [Allogene Therapeutics](#), retrieved on 14.01.2019

C.R. Bard ⁶⁸ Headquarters Employees Corporate Family Annual Sales Total Assets	New Providence, New Jersey 16.000 384 companies 3.7 billion US\$ 5.5 billion US\$
Elekta ⁶⁹ Headquarters Employees Corporate Family Annual Sales Total Assets	Atlanta, Georgia 100 49 companies 110 million US\$ 42 million US\$
Flatiron Health ⁷⁰ Headquarters Employees Corporate Family Annual Sales Total Assets	New York, New York 400 470 companies 1.2 billion US\$ N/A
Guardant Health ⁷¹ Headquarters Employees Corporate Family Annual Sales Total Assets	Redwood City, California 348 N/A 49 million US\$ 362 million US\$
Nanthealth ⁷² Headquarters Employees Corporate Family Annual Sales Total Assets	Culver City, California 864 9 companies 86 million US\$ 411 million US\$

⁶⁸ Source: Hoovers (2019), [C.R. Bard](#), retrieved on 14.01.2019

⁶⁹ Source: Hoovers (2019), [Elekta](#), retrieved on 14.01.2019

⁷⁰ Source: Hoovers (2019), [Flatiron Health](#), retrieved on 14.01.2019

⁷¹ Source: Hoovers (2019), [Guardant Health](#), retrieved on 18.01.2019

⁷² Source: Hoovers (2019), [Nanthealth](#), retrieved on 18.01.2019

Varian Medical Systems ⁷³	
Headquarters	Palo Alto, California
Employees	6.600
Corporate Family	72 companies
Annual Sales	2.9 billion US\$
Total Assets	3.1 billion US\$

1.4.2. Associations

Shown in the table down below are prominent associations for oncology. ⁷⁴

Table 10: Associations for oncology

Associations	Links
American Society of Clinical Oncology	ASCO
Community Oncology Alliance	COA
Society of Surgical Oncology	SSO
American Society for Radiation Oncology	ASTRO
American Society of Blood and Marrow Transplantation	ASBMT
American Association of Cancer Research	AACR
American Cancer Society	ACS
National Cancer Institute	NCI
National Comprehensive Cancer Network	NCCN

⁷³ Source: Hoovers (2019), [Varian Medical Systems](#), retrieved on 18.01.2019


⁷⁴ APAO (2019), [Oncology Professional Organizations](#), retrieved on 18.01.2019

1.5. Orthopedics

1.5.1. Medical Technological Market for Orthopedics

The orthopedic device market is expected to grow in the coming years. A special focus is laid on reducing diseases that come with old age as shown in Figure 10. The rise in osteoporosis, osteoarthritis, and musculoskeletal disorders due to old age is a driving factor for the orthopedic device industry. Orthopedics also covers the surge of surgery that deals with musculoskeletal system conditions such as trauma, sport injuries, degenerative diseases, infections, and tumors. Younger individuals in their 40s and 50s undertake orthopedic surgeries most commonly due to injuries and in need of orthopedic implants. The orthopedic sector is one of the fastest growing segments in the US medical device industry. The orthopedic implants and devices market forms a substantial part of the overall medical device industry and accounts for 125 billion US\$ made in revenue.

Figure 10: Share of Americans who underwent orthopedic treatment in the last 3 years in 2018, by age⁷⁵

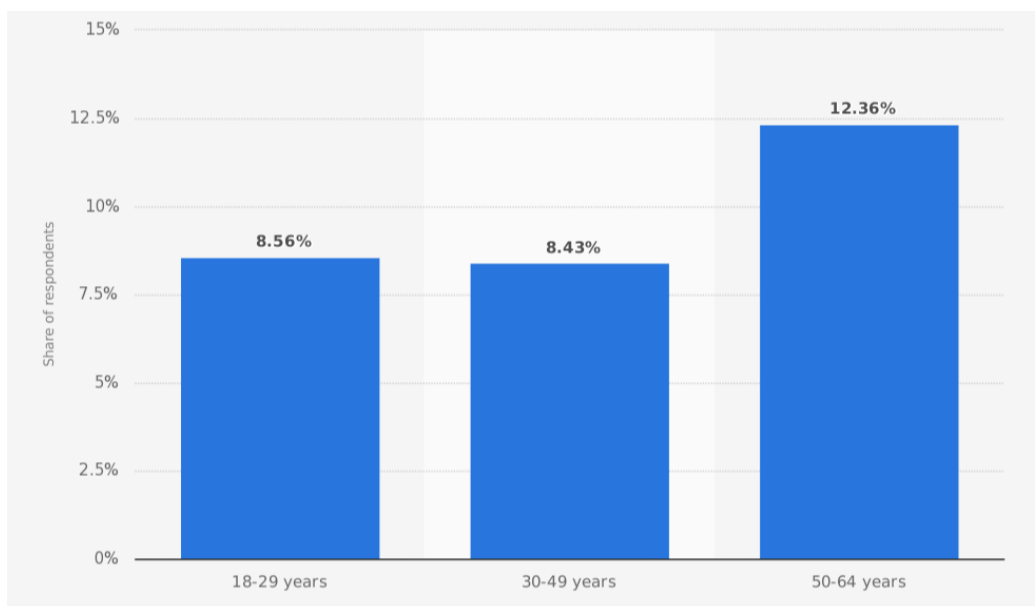


⁷⁵ Source: Statista (2018), [Share of Americans who underwent orthopedic treatment in the last 3 years in 2018, by age](#), retrieved on 18.01.2019

1.5.1.1. Market Size & Growth

The US orthopedic device market was valued at over 20 billion US\$ in 2016. The US orthopedic device market holds over 90% of regional revenue. It is projected to produce 25 billion US\$ in revenue by 2024.⁷⁶ Traditional medical device companies display the biggest market share in the orthopedic sector.

Figure 11: Global top 10 companies based on orthopedic medical technology market share in 2017 and 2024.⁷⁷

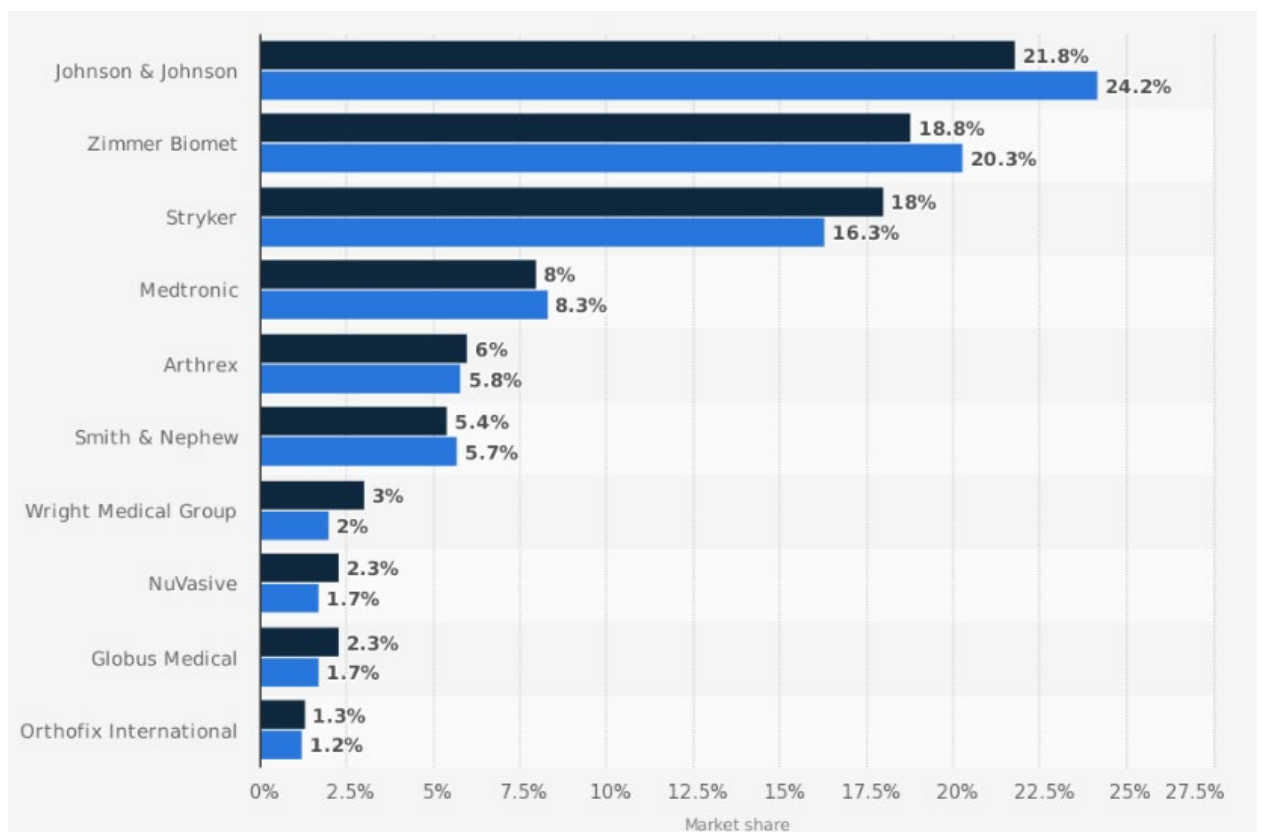

The top 10 leading medical companies for orthopedics, as shown in Figure 11, account for over 90 % of the market. However, the industry has reached a maturity stage, since the supply for orthopedics implants and devices has exceeded the demand.

⁷⁶ Source: Global Markets Insight (2017), [Orthopedic Devices Market Size By Product](#), retrieved 18.01.2019

⁷⁷ Source: Statista (2018), [Global top 10 companies based on orthopedic medical technology market share in 2017 and 2024](#), retrieved on 18.01.2019

1.5.1.2. US companies for Orthopedics

The table below displays the major manufacturers for orthopedics in the US market in alphabetical order.

Table 11: US companies for Orthopedics

Companies	Key figures
Arthrex ⁷⁸	
Headquarters	Naples, Florida
Employees	1.200
Corporate Family	28 companies
Annual Sales	426 million US\$
Total Assets	1.3 million US\$
Globus Medical ⁷⁹	
Headquarters	Audubon, Pennsylvania
Employees	1.400
Corporate Family	9 companies
Annual Sales	635 million US\$
Total Assets	1.2 billion US\$
Johnson & Johnson ⁸⁰ (DePuy Products)	
Headquarters	Warsaw, Indiana
Employees	12.000
Corporate Family	941 companies
Annual Sales	1.3 billion US\$
Total Assets	N/A
Medtronic ⁸¹	
Headquarters	Minneapolis, Minnesota
Employees	49.000
Corporate Family	611 companies

⁷⁸ Source: Hoovers (2019), [Arthrex](#), retrieved on 14.01.2019

⁷⁹ Source: Hoovers (2018), [Globus Medical](#), Inc., retrieved on 18.01.2019

⁸⁰ Source: Hoovers (2018), [Johnson & Johnson](#), retrieved on 18.01.2019

⁸¹ Source: Hoovers (2018), [Medtronic](#), retrieved on 18.01.2019

Annual Sales	19 billion US\$
Total Assets	55 billion US\$

[NuVasive](#)⁸²

Headquarters	San Diego, California
Employees	2.600
Corporate Family	19 companies
Annual Sales	1 billion US\$
Total Assets	1.6 billion US\$

[Orthofix](#)⁸³

Headquarters	Lewisville, Texas
Employees	525
Corporate Family	11 Companies
Annual Sales	122 million US\$
Total Assets	N/A

[Stryker Corporation](#)⁸⁴

Headquarters	Portage, Michigan
Employees	33.000
Corporate Family	241 companies
Annual Sales	12 billion US\$
Total Assets	22 billion US\$

[Wright Medical Group](#)⁸⁵

Headquarters	Memphis, Tennessee
Employees	989
Corporate Family	55 companies
Annual Sales	298 million US\$
Total Assets	1.1 billion US\$

[Zimmer Biomet Holdings](#)⁸⁶

Headquarters	Warsaw, Indiana
Employees	18.000
Corporate Family	106 Companies

⁸² Source: Hoovers (2018), [NuVasive](#), retrieved on 18.01.2019

⁸³ Source: Hoovers (2018), [Orthofix](#), retrieved on 18.01.2019

⁸⁴ Source: Hoovers (2018), [Stryker Corporation](#), retrieved on 18.01.2019

⁸⁵ Source: Hoovers (2018), [Wright Medical Group](#), retrieved on 18.01.2019

⁸⁶ Source: Hoovers (2018), [Zimmer Biomet Holdings](#), retrieved on 18.01.2019

Annual Sales	7.8 billion US\$
Total Assets	25 billion US

1.5.2. Associations for Orthopedic

Shown in the table down below are prominent associations for orthopedic.

Table 12: Associations for orthopedic

Associations	Links
American Academy of Orthotics and Prosthetics	<u>AAOP</u>
American Association for Surgery of Trauma	<u>AAST</u>
American Association of Hip and Knee Surgeons	<u>AAHKS</u>
American Association of Neurological Surgeons	<u>AANS</u>
American Association of Orthopaedic Executives	<u>AAOE</u>
American Association of Orthopaedic Surgeons	<u>AAOS</u>
American Association of Tissue Banks	<u>AATB</u>
American College of Surgeons	<u>ACS</u>
American Orthopaedic Association	<u>AOA</u>
American Orthopaedic Foot and Ankle Society	<u>AOFAS</u>
American Orthopaedic Society for Sports Medicine	<u>AOSSM</u>
American Shoulder and Elbow Surgeons	<u>ASES</u>
American Society for Surgery of the Hand	<u>ASSH</u>
American Society of Bone and Mineral Research	<u>ASBMR</u>
American Society of Orthopaedic Professionals	<u>ASOP</u>
American Spinal Injury Association	<u>ASIA</u>

2. Regulatory affairs

2.1. US import regulation; general overview

All foreign items brought to the US have to meet the import requirements of the US Customs and Border Protection (CBP). Thus every item crossing the border is subject to customs clearance and duties (unless specifically exempted).

The US customs regulations are generally stated in section 19 of the US Code. Most of the specific regulations, however, are put down in section 19 of the Code of Federal Regulations (CFR - "Customs Duties"). Other responsible authorities besides the CBP are the US Immigration and Customs Enforcement (within the Department of Homeland Security, (DHS)), Department of the Treasury, United States International Trade Commission (ITC) and the International Trade Administration (ITA).⁸⁷

2.1.1. Trade policy frame work

Besides being part of the World Trade Organization (WTO) the US has free trade agreements with many countries, notably USMCA, the United States-Mexico- Canada Agreement.⁸⁸ The WTO oversees most global trade in goods and services and provides arbitration in case of disputes. Free Trade Agreements lead to eased conditions, specifically elimination or progressive reduction of tariffs on qualified goods.⁸⁹

2.1.2. Customs procedure

CBP does not require an importer to have a license or permit, but other agencies may require such documents or other certification, depending on the goods that are being imported.⁹⁰

In most cases, customs business should be processed through a customs broker, acting on behalf of the importers needs. A valid customs broker license is mandatory.

Upon formal entry, the importer has to transmit an identification number to the authorities. In case of a resident importer (companies located in the U.S) this number is the IRS business registration number ("Internal Revenue Service employer identification number") or Social Security number. If the importer is a non-resident importer, CBP will assign an "Importer Identification Number" which will be valid for future customs business as well. Customs declaration in the US can only be made by the "Importer of Record" (IOR) meaning the owner, purchaser or customs broker.⁹¹

⁸⁷ Source: GTAI (2018), [Merkblatt über gewerbliche Wareneinfuhren-USA](#), retrieved on 08.01.2019

⁸⁸ Source: USTR (2018), [United States-Mexico-Canada Agreement](#), retrieved on 08.01.2019

⁸⁹ Source: GTAI (2018), [Merkblatt über gewerbliche Wareneinfuhren und Basiswissen Einfuhr](#), retrieved on 08.01.2019

⁹⁰ Source: USgov (2018), [Importing and Exporting](#), retrieved on 08.01.2019

⁹¹ Source: GTAI (2018), [Merkblatt über gewerbliche Wareneinfuhren – USA](#), retrieved on 10.01.2019

2.1.3. Import duties

Import duties are taxes paid for goods that are transported across international borders. In case of a trade agreement, however, some countries and goods are exempt from duties. These goods still have to be declared. The customs tariffs are defined in the Harmonized Tariff Schedule of the United States (HTSUS) issued by the United States International Trade Commission. All goods that enter the United States are categorized according to the Harmonized Tariff Schedule. Besides those tariffs, certain products can be subject to additional duties.⁹²

Example: Since July 2018, several products with origin from China are charged 25 percent of additional duties besides the basic customs duties.⁹³

2.1.4. Import bans & restrictions

Prohibitions or restrictions apply to the import of certain goods into the US depending on various factors, e.g. the country of origin or product type.

Import restrictions limit the entry of certain products into the US. An example of a category, which is limited by such restrictions, is medical devices.⁹⁴

Manufacturers must be very cautious regarding country of origin requirements and potential for additional duties.

According to customs and international trade law expert Mariana del Rio Kostenwein, it is advisable to conduct an analysis of the country of origin of the device to ensure the products are e.g. not considered to be "Made in China" by CBP and subject to additional duties.⁹⁵

2.1.5. Excuse: export restriction (EU)

Export control law restrictions may apply to goods, countries or persons for various reasons.⁹⁶

The export of dual-use items is subject to control mainly carried out on the basis of European regulation (EC) No. 428/2009. Dual-use items are goods, software and technology that can be used for both civilian and military applications. The EU controls the export, transit and brokering of dual-use items, so the EU can contribute to international peace and security and prevent the proliferation of Weapons of Mass Destruction (WMD).⁹⁷ The relevant items are listed in Annex I of the regulation. Despite the fact that

⁹² Source: CBP, [Customs Duty Information](#), retrieved on 08.01.2019

⁹³ Source: GTAI (2018), [Merkblatt über gewerbliche Wareneinführen und Basiswissen Einfuhr](#), retrieved on 10.01.2019

⁹⁴ Source: GTAI (2018), [Merkblatt über gewerbliche Wareneinführen und Basiswissen Einfuhr](#), retrieved on 10.01.2019

⁹⁵ Interview with Marina del Rio Kostenwein, Partner at Simon Gluck & Kane LLP, on 08.01.2019

⁹⁶ Source (2018): Zoll, [Wirtschaft und Sicherheit](#), retrieved on 10.01.2018.

⁹⁷ Source: European Commission (2018), [Dual-use trade controls](#), retrieved on 10.01.2019

medical devices may contain sensitive technology, they are not listed in the Annex or subject to control otherwise. In fact they are explicitly exempt according to the Annex.

2.2. Import of medical devices; specific regulations

Medical devices that are imported into the US must not only meet CBP requirements but also the regulations of the FDA. Products not meeting the FDA regulatory requirements may be detained upon entry, even if the product is authorized for marketing in another country.

Said requirements include the registration of establishment, listing of devices or premarket submissions among others.

At the beginning of the import process the importer or filer has to submit the necessary information to the local CBP office. The entry submission should contain the necessary information in order to identify the product (especially name of device & product code) and also contain the appropriate information demonstrating that the product is in compliance with FDA regulations. Upon entry into the U.S, FDA may examine certain devices to confirm all the requirements are being fulfilled. In this case there will be a notice given by FDA ("Notice of FDA Action").⁹⁸

According to expert Mariana del Rio Kostenwein, the common legal issues European companies may face when first entering the US market include: determining whether or not the product is a medical device; in case of a medical device, determining the device classification; if required, preparing and submitting the necessary application to FDA for clearance and approval; determining device labelling as well as protecting the device's intellectual property. Ms. Del Rio Kostenwein also explained that although the Transatlantic Trade and Investment Partnership (TTIP) did not come into effect, the US and EU are discussing harmonization, which would make market entry easier for European medical device manufacturers.⁹⁹

2.2.1. FDA's medical device regulation

Medical devices (radiation emitting or non-radiation emitting) or other products that emit radiation imported by foreign manufacturers also have to comply with applicable US regulations prior, during and after the import into the US or its territories. Those devices or products emitting radiation must meet FDA regulatory requirements in order to be imported. Regulatory approvals from other countries are not recognized by the FDA.¹⁰⁰

⁹⁸ Source: FDA (2018), [Importing into the U.S.](#), retrieved on 10.01.2019

⁹⁹ Interview with Marina der Rio Kostenwein, Partner at Simon Gluck& Kane LLP, on 08.01.2019

¹⁰⁰ Source: FDA (2018), [Importing into the U.S.](#), retrieved on 10.01.2019

2.2.1.1. Statutory framework: FD&C Act, 21 CFR Parts 1-58, 800-1299; CDRH

There are several regulations which need to be observed when importing and introducing medical devices to the US market.

Federal Food, Drug, and Cosmetic Act (FD&C Act): This Act outlines the legal framework within which FDA operates. It allows regulating both medical devices (emitting radiation or not) and electronic radiation-emitting products. The FDA's level of control over these products is determined by this law, enabling them to develop, publish and implement regulations.¹⁰¹

Code of Federal Regulations (CFR): This codification contains the general and permanent rules. It represents the broad areas subject to the Federal Regulation. Most of the FDA's medical device and radiation-emitting product regulations are stated in Title 21 CFR Parts 800-1299. These regulations cover various aspects of design, clinical evaluation, manufacturing, packaging, labeling and post market surveillance of medical devices.¹⁰²

Center for Devices and Radiological Health (CDRH): This institution is responsible for regulating companies who manufacture, repackage, relabel and/or import medical devices sold in the US. It also sets the regulations regarding radiation-emitting electronic products (medical and non-medical).¹⁰³

2.2.1.2. Regulated products

The FDA regulates medical devices in order to assure the safety and effectiveness of those devices. Additionally, it develops and carries out a national program (by the CDRH) in order to control unnecessary exposures to and assure safe use of ionizing and non-ionizing radiation-emitting electronic products.

In order to know whether a product will be regulated by FDA, it is necessary to determine whether the product is defined as a medical device according to section 201(h) or a radiation-emitting product, as defined in Section 531 of the FD&C Act or both. If the product meets these definitions, the FD&C Act applies, meaning the regulatory requirements set by the FDA have to be fulfilled.¹⁰⁴

¹⁰¹ Source: FDA (2018), [What is the difference between the Federal Food, Drug, and Cosmetic Act \(FD&C Act\), FDA regulations, and FDA guidance?](#), retrieved on 17.01.2019

¹⁰² Source: FDA (2018), [Code of Federal Regulations \(CFR\)](#), retrieved on 16.01.2019

¹⁰³ Source: FDA (2018), [Overview of Device Regulation](#), retrieved on 16.01.2019

¹⁰⁴ Source: FDA (2018), [Overview of Device Regulation](#), retrieved on 27.01.20189

Medical devices involved in the collection, processing, testing, screening, manufacture and administration of blood, blood components and human tissue and cellular products are, however, specifically regulated by the Center for Biologics Evaluation and Research (CBER).¹⁰⁵

2.2.1.2.1. Medical device and radiation emitting device

Medical devices vary from simple bandages to complex programmable pacemakers with micro-chip technology and laser surgical devices. Furthermore, in vitro diagnostic products fall into this category, i.e. general-purpose lab equipment, reagents and test kits, which may include monoclonal antibody technology. In addition, certain electronic radiation emitting products with medical applications and claims can be defined as medical devices, such as diagnostic ultrasound products or x-ray machines.¹⁰⁶

2.2.1.2.2. Medical device accessory

An accessory is a finished device intended to supplement, support or increase the performance of one or more parent devices. Parent devices in turn are finished devices whose performance is supplemented, supported or increased by one or more accessories. A device is considered an accessory if promotional material, labeling or other evidence of intended use show that the device is designed to supplement, support or extend another device.¹⁰⁷

Example: An infusion pump system will usually include a stand and an infusion pump. The performance of the infusion pump is supported by the stand by allowing the infusion pump to hold medications and liquids in comfortable reach of the patient or caregiver and at a suitable height. In this example, the infusion pump would be considered the parent device and the stand would be considered the accessory to the infusion pump.

Articles that do not meet the definition of an accessory cannot be treated as such even though they may be used in connection with a device.

Example: A mobile smartphone would not be considered an accessory after having downloaded a medical app, since the smartphone was not specifically determined for use with the medical device.¹⁰⁸

2.2.1.3. Control standards and tools – overview

General Controls are the basic rules of the Medical Device Amendments to the FD&C Act. These rules provide the FDA with the means of regulating devices to ensure their safety and effectiveness. They apply

¹⁰⁵ Source: FDA (2018), [CBER Regulated Products](#), retrieved on 08.01.2019

¹⁰⁶ Source: FDA (2018), [Products and Medical Procedures](#), retrieved on 08.01.2019

¹⁰⁷ Source: FDA (2018), [Medical Device Accessories](#), retrieved on 09.01.2019

¹⁰⁸ Source: FDA (2018), [Medical Device Accessories](#), retrieved on 09.01.2019

to all medical devices and include provisions relating to misbranding, device registration and listing, premarket notification, banned devices and notifications.

The Amendments established three regulatory classes for medical devices. The devices are classified according to the degree of difficulty in assuring their safety and effectiveness. Regulatory control increases from Class I to Class III.¹⁰⁹

Class I (synonymous with General Control) is the least rigid of the three device classes provided in the Amendments. Placing a device in Class I, the FDA has to conclude that there is sufficient information available about the device. Devices in said Class are not subject to the restrictions of Class II or III. Moreover, those devices are not intended for use in supporting or sustaining life or to be of substantial importance in preventing impairment to human health.

The General Controls are applicable to all devices regardless of their classification. They are, however, the only level of controls that apply to Class I devices.¹¹⁰

2.2.1.3.1. Device classification (Class I, II, III)

As already mentioned, devices are classified according to the degree of difficulty in assuring their safety and effectiveness. In order to do so, the FDA has determined classifications for about 1,700 different generic types of devices and categorized them into 16 medical specialties, the so-called "panels" (e.g. cardiovascular devices).¹¹¹ Each of these generic types of devices is assigned to one of three regulatory classes based on the level of control. Classification is therefore risk based, confirms expert Mariana del Rio Kostenwein. That is to say the risk the device poses to the patient or the user is a main factor in the assignment of the classification. Devices with the lowest risk are appointed to Class I while those with the greatest risk are appointed to Class III.

The three classes are the following:

1. Class I: General Controls
 - With Exemptions
 - Without Exemptions
2. Class II: General Controls and Special Controls
 - With Exemptions
 - Without Exemptions
3. Class III: General Controls and Premarket Approval (PMA)

¹⁰⁹ Source: FDA (2018), [PMA Approvals](#), retrieved on 08.01.2019

¹¹⁰ Source: FDA (2018), [General Controls for Medical Devices](#), retrieved on 09.01.2019

¹¹¹ Source: FDA (2018), [Device Classification Panels](#), retrieved on 08.01.2019

Among other criteria, the Class being assigned is decisive for the type of premarketing submission/ application required for FDA clearance to the market.

In case the device is classified as Class I or II (without an exemption) a 510(k) submission will be obligatory for marketing. If the device is classified as exempt it is subject to the limitations on exemptions. These limitations of device exemptions are covered under Section 21 CFR.

For Class III devices, a premarket approval application (PMA) is necessary unless the device is a preamendments device (on the market prior to the passage of the medical device amendments in 1976, or substantially equivalent to such a device) and PMA's have not been called for. If so, a 510(k) submission is required. These Class III devices are therefore the most difficult devices to get approved by the FDA says expert Mariana del Rio Kostenwein. She further explained that the PMA process is more time consuming and costly than the requirements for Class II devices.¹¹²

The classification of a device is based on the intended use as well as the indication for use. These indications for use are usually taken from the device's labeling, but can also be stated orally during sale of the product. Example: A scalpel's intended use is to cut tissue. A subset of intended use arises when a more specialized indication is added in the device's labeling such as, "for making incisions in the cornea".

In order to determine the device's appropriate classification, the regulation number is mandatory. This number can either be requested in the classification database or directly in the listing for the specific panel, confirms expert Mariana del Rio Kostenwein.¹¹³

Most medical devices can be classified by finding the matching description of the device in Title 21 CFR, Parts 862-892.¹¹⁴

2.2.1.3.2. Quality System (QS) regulation; CGMP & design controls

In order to ensure that the products meet the applicable requirements and specifications, the manufacturers have to establish and follow certain quality systems.

The quality systems for FDA-regulated products, such as medical devices are known as current good manufacturing practices (CGMPs). The respective CGMP requirements for devices are codified under 21 CFR part 820.¹¹⁵

¹¹² Interview with Marina der Rio Kostenwein, Partner at Simon Gluck& Kane LLP, on 08.01.2019

¹¹³ Interview with Marina der Rio Kostenwein, Partner at Simon Gluck& Kane LLP, on 08.01.2019

¹¹⁴ Source: FDA (2018), [Classify Your Medical Device](#), retrieved on 10.01.2019

¹¹⁵ Source: FDA (2018), [Quality System \(QS\) Regulation/Medical Device Good Manufacturing Practices](#), retrieved on 08.01.2019

The FDA has now revised these CGMPs and incorporated them into a quality system regulation (QS) in order to achieve consistency with quality systems worldwide and giving device manufacturers greater flexibility in managing quality requirements (61 FR 52602). The QS regulations include requirements regarding methods, facilities and controls used in the proof of designing, manufacturing, packaging, labeling, storing, installing and servicing of medical devices intended for human use.¹¹⁶

Since the QS regulations have to cover various types of devices, they only establish a framework, rather than specific rules for each product. This framework has to be followed by all manufacturers meaning they have to develop and follow procedures and fill in the details required to determine the current state-of-the-art manufacturing for the specific device.

These rules are applicable to finished device manufacturers who intend to commercially distribute medical devices. The definition of a finished device is found in 21 CFR 820.3(l) (any device or accessory to any device that is suitable for use or capable of functioning, whether or not it is packaged, labeled or sterilized).

Certain components such as blood tubing and diagnostic x-ray components are considered to be finished devices because they are accessories to finished devices. A manufacturer of accessories is subject to the QS regulation.

However, certain types of medical devices do not have to fulfill the CGMP requirements. These devices are exempted by FDA classification regulations (21 CFR 862 to 892).¹¹⁷

An important component of the QS regulations are design controls. They describe an interrelated set of practices and procedures that are incorporated into the design and development process. Design controls make systematic assessment of the design an integral part of development.¹¹⁸

2.2.1.3.3. Medical device reporting (MDR)

The Medical Device Reporting (MDR) regulation (21 CFR 803) contains mandatory requirements for manufacturers, importers and device user facilities to report certain device-related adverse events and product

¹¹⁶ Source: GovInfo (N.A.), [Federal Register Volume 61, Issue 195 \(October 7, 1996\)](#), retrieved 14.01.2019

¹¹⁷ Source: FDA (2018), [Quality System \(QS\) Regulation/Medical Device Good Manufacturing Practices](#), retrieved on 08.01.2019.

¹¹⁸ Source: FDA (1997), [Design Control Guidance for Medical Device Manufacturers](#), retrieved on 08.01.2019

problems to the FDA.¹¹⁹ It functions as a post-market surveillance tool in order to monitor device performance, detect potential device-related safety issues and contribute to benefit-risk assessments of these products. The goal is to detect and correct problems in a timely manner.¹²⁰

Manufacturers: A report filed by the manufacturer is required when they learn that any of their devices may have caused or contributed to a death or serious injury (key terms are defined in 21 CFR 803.3.). Once the manufacturer becomes aware of the fact that their device has malfunctioned and would be likely to cause or contribute to a death or serious injury if the malfunction were to recur, a report has to be filed as well.

Importers: Importers are required to report to the FDA and the manufacturer when they learn that one of their devices may have caused or contributed to a death or serious injury. If an importer learns their imported devices have malfunctioned and would be likely to cause or contribute to a death or serious injury if the malfunction were to recur, they are only required to notify the manufacturer.

Device User Facilities (i.e. hospital, ambulatory surgical facility): User facilities have to report a suspected medical device-related death to the FDA and the manufacturer. They also have to report a medical device-related serious injury to the manufacturer (or to the FDA if the medical device manufacturer is unknown). However, no report is needed in case of a device malfunction, but such incidents can be reported on a voluntary basis to the FDA.¹²¹

2.2.1.3.4. Label & Labeling requirements

The general labeling requirements for medical devices are stated in 21 CFR Part 801. These regulations specify the minimum requirements for all devices. Additional regulations can be found in Parts 809, 812, 820, 830.¹²²

Labeling in this context means providing proper information about name and place of the business, the intended use of the device as well as adequate directions for use, meaning a directive for safe use.

A device is considered misbranded if it makes a false or misleading statement with respect to another device, drug, food or cosmetic.

Exemptions may be granted due to lack of sufficient space for the required labeling if labelling space is not depleted by including non-required information. The existing label space may not be used for any

¹¹⁹ Source: FDA (2018), [Mandatory Reporting Requirements: Manufacturers, Importers and Device User Facilities](#), retrieved on 08.01.2019

¹²⁰ Source: FDA (2018), [Medical Device Reporting \(MDR\)](#), retrieved on 10.01.2019

¹²¹ Source: FDA (2018), [Medical Device Reporting \(MDR\)](#), retrieved on 10.01.2019

¹²² Source: FDA (2018), [General Device Labeling Requirements](#), retrieved on 08.01.2019

representations in a foreign language. All labeling shall be in English with the exception of products distributed solely within Puerto Rico or a US territory where the predominant language is other than English. If any representation on the device label or labeling appears in a foreign language, then all required labeling shall also appear in that foreign language.¹²³

Other relevant regulations are stated in the FD&C Act, specifically in Section 201(k) and Section 201(m).¹²⁴

2.2.1.4. Premarket Submission

After having classified a device, there are several different premarket submissions depending on the applicable regulation. The following are the most common types of premarket submissions.¹²⁵

The FDA has developed several types of resources to assist with a premarket submission. For more information please visit the FDA's website.¹²⁶

2.2.1.4.1. 513(g) Application

The 513(g) submissions provide aid clarifying the FDA's view about the classification and the regulatory requirements that may be applicable to a device. A submission therefore constitutes a request for information. In order to receive all the necessary information, the submission should outline the characteristics of the device. The FDA will evaluate the information within 60 days and issue a ruling on how the device should be classified.¹²⁷

For more details visit the FDA 513(g) guidance document.¹²⁸

2.2.1.4.2. 510(k) submission – Premarket notification

Most Class II but also some Class I devices require a 510(k) submission. This notification requires the manufacturer to demonstrate that the new device is "substantially equivalent" to a predicate device in terms of intended use, technological characteristics and performance testing.¹²⁹ The notification has to be sent to the FDA at least 90 days in advance for review, confirms expert Mariana del Rio Kostenwein. This way, the FDA is able to determine whether the device is equivalent to a device already placed into one of the three classification categories, and "new"

¹²³ Source: FDA (2018), [General Device Labeling Requirements](#), retrieved on 08.01.2019

¹²⁴ Source: FDA (2018), [Device Labeling](#), retrieved on 10.08.2019

¹²⁵ Source: FDA (2018), [How to Study and Market Your Device](#), retrieved on 17.01.2019

¹²⁶ Source: FDA (2018), [Device Advice: Comprehensive Regulatory Assistance](#), retrieved on 08.01.2019

¹²⁷ Source: FDA (2018), [Guidance for Industry and Food and Drug Administration Staff](#), retrieved on 18.01.2019

¹²⁸ Source: FDA (2018), [Guidance for Industry and Food and Drug Administration Staff](#), retrieved on 18.01.2019

¹²⁹ Source: FDA (2018), [How to Study and Market Your Device](#), retrieved on 07.01.2019

unclassified devices can be properly identified. In case a medical device manufacturer intends to introduce a device into commercial distribution for the first time or reintroduce a significantly modified device (affecting safety and effectiveness), are required to submit a premarket notification.¹³⁰

For additional information visit the FDA's Device Advice Premarket Notification 510(k).¹³¹

2.2.1.4.3. Premarket approval (PMA)

PMA poses the most stringent type of premarket submission (application under section 515). It is used to evaluate the safety and effectiveness of only Class III medical devices. A premarket approval (PMA) is the FDA's process of scientific and regulatory review.

Because of the high level risk associated with Class III devices, general and special controls are not sufficient to assure safety and effectiveness of these devices.

Some Class III preamendment devices may require a Class III 510(k) submission.

The applicant has to receive FDA approval of their PMA application prior to marketing the device. An approved PMA is a private license granting the applicant permission to market the device.

According to FDA regulations, the review timeframe for PMAs is 180 days, though in most cases the period is longer, says expert Mariana del Kostenwein.¹³²

2.2.1.4.4. De Novo classification

The De Novo process provides a means for classifying a new device without a valid predicate but already providing reasonable assurance of safety and effectiveness for the intended use through general and or special controls.

De Novo classification is a risk-based classification process. Devices being classified into Class I or II through this process may be marketed and also used as predicated for future premarket notifications, 510(k) submissions.¹³³

2.2.1.4.5. Humanitarian Device Exemption (HDE)

For a device to be eligible for an HDE, a sponsor has to obtain designation as a Humanitarian Use Device (HUD). A HUD describes a

¹³⁰ Source: FDA (2018), [510\(k\) Clearances](#), retrieved on 10.01.2019

¹³¹ Source: FDA (2018), [Premarket Notification 510\(k\)](#), retrieved on 08.01.2019

¹³² Source: FDA (2018), [Premarket Approval \(PMA\)](#), retrieved on 09.01.2019

¹³³ Source: FDA (2018), [Evaluation of Automatic Class III Designation \(De Novo\)](#), retrieved on 08.01.2019

medical device intended to benefit patients in the treatment or diagnosis of rare diseases.

HDE in turn describes a marketing application for an HUD. It states an exemption from the effectiveness requirements of Sections 514 and 515 of the FD&C Act and is subject to certain profit and use restrictions.¹³⁴

2.2.1.4.6. Investigational Device Exemption (IDE) for clinical studies

An investigational device exemption (IDE) allows for an investigational device to be used in a clinical study in order to collect safety and effectiveness data. Clinical studies are mostly conducted to support a Premarket Approval. In terms of 510(k) submission there are only few requiring clinical data to support the application.

Investigational use includes clinical evaluation of certain modifications or new intended uses of legally marketed devices.

All clinical evaluations of investigational devices require an approved IDE before the study is initiated.

Following an approved IDE, a device can be shipped lawfully for the purpose of its conducting investigations without fulfilling other requirements of the FD&C Act which would usually apply with devices in commercial distribution. Accordingly, there is no need to submit a PMA or 510(k) and also no registration of the establishment or the device.¹³⁵

2.2.1.5. Registration and Listing

An annual registration with the FDA is required for all establishments involved in commercial distribution within the US, including those distributions imported for export only. According to Title 21 CFR Part 807 most of said establishments are also required to list the devices as well as the activities performed on those devices at the establishment. Based on the different types of activities performed, the requirements for registration vary. Moreover, different requirements apply for domestic and foreign establishments.

For more details, visit the FDA's website.¹³⁶

2.2.1.5.1. Establishment registration (initial, annual)

The obligation to register applies to all establishments. This includes all owners or operators of places of business, thus allowing the FDA to obtain the location of the establishment. By knowing where devices are made, the US is better able to prepare for and respond to public health emergencies.¹³⁷ All device establishments need to complete their annual

¹³⁴ Source: FDA (2018), [Humanitarian Device Exemption](#), retrieved on 08.01.2019

¹³⁵ Source: FDA (2018), [Device Advice: Investigational Device Exemption \(IDE\)](#), retrieved on 08.01.2019

¹³⁶ Source: FDA (2018), [Who Must Register, List and Pay the Fee](#), retrieved on 08.01.2019

¹³⁷ Source: FDA (2018), [Device Registration and Listing](#), retrieved on 08.01.2019

registration for each fiscal year between October 1st and December 31st.¹³⁸

2.2.1.5.2. Medical device listing

Besides the requirement to register most of the establishments are also expected to list the devices manufactured at the establishment as well as the activities performed on them. In case a certain device requires premarket approval before being marketed in the U.S, the owner or operator should provide the FDA with a premarket submission number. Both registration and listing must be submitted electronically with an own account using the FDA's unified system and listing module.¹³⁹

2.2.1.5.3. Fees

The FDA will collect an annual establishment registration fee for device establishments. Payment must be made in order to register the establishment.¹⁴⁰ For 2019 the fee amounts to \$4,884.¹⁴¹

2.2.2. Supplementing & displaced regulations

Besides the FDA, there are other agencies, on a federal and state level, regulating the market entry of medical devices. Accordingly, there can be some jurisdictional overlap between the FDA and other agencies in terms of some aspects or components of a medical device.

2.2.2.1. Federal level (FCC, CPSC, OSHA)

Federal Communications Commission (FCC):

The purpose of the FCC is to oversee the use of the public Radio Frequency (RF) spectrum within which RF wireless technologies operate. RF wireless medical devices perform at least one function that utilizes wireless RF communication such as Wi-Fi or Bluetooth to support health care delivery.

Example: controlling and programming a medical device or monitoring patients remotely.¹⁴²

The FDA's policies on wireless medical devices are coordinated with the FCC and provide medical device manufacturers with more predictability and a better understanding of regulatory requirements for medical devices that utilize these technologies.¹⁴³ In fact there is a Memorandum of Understanding in which the agencies agree to work together to

¹³⁸ Source: FDA (2018), [Important Reminders about Registration and Listing](#), retrieved on 09.01.2019

¹³⁹ Source: FDA (2018), [Device Registration and Listing](#), retrieved on 09.01.2019

¹⁴⁰ Source: FDA (2018), [Payment Process](#), retrieved on 09.01.2019

¹⁴¹ Source: FDA (2018), [Device Registration and Listing](#), retrieved on 09.01.2019

¹⁴² Source: FDA (2018), [Wireless Medical Devices](#), retrieved on 08.01.2019

¹⁴³ Source: FDA (2018), [Wireless Medical Devices](#), retrieved on 08.01.2019.

promote a health information technology (IT) framework that promotes innovation, protects patient safety and avoids regulatory duplication.¹⁴⁴

Consumer Product Safety Commission (CPSC):

The responsibility of the CPSC is to protect the public from unreasonable risks of injury associated with consumer products. In order to accomplish said task the Commission is authorized, among other things, to issue consumer product safety standards or to establish requirements for warnings and instructions. In that regard the commission has jurisdiction over many types of consumer products. However, some types of consumer products are covered by other Federal agencies, depending on the particular class of "consumer product". A Memorandum of Understanding delineates the respective areas of jurisdiction between the two agencies.¹⁴⁵ In terms of jurisdiction of medical devices, the FDA has the sole jurisdiction.¹⁴⁶

Occupational Safety and Health Administration of the Department of Labor (OSHA):

OSHA is required to enforce the Occupational Safety and Health Act of 1970 (OSH Act), under which employers are responsible for providing safe and healthful workplaces for their employees. Its role is therefore to assure these conditions by setting and enforcing standards, and providing training, education and assistance.¹⁴⁷

The requirements of the FDA to obtain market clearance for medical devices are unrelated to these OSHA requirements. OSHA's jurisdiction concerns protecting the employees (physicians, nurses, medical technicians) who use the device. The jurisdiction of the FDA on the other hand concerns testing the safety and efficacy of medical devices with regard to the manner in which these devices are used (i.e., medical safety of patients). Typically, the FDA evaluates the extent to which the devices meet the purported treatment objectives in a manner that does not endanger the patient, while OSHA is responsible for ensuring that the equipment is safe for use by employees in the workplace.

Moreover, the FDA regulates the manufacturers of medical devices, while OSHA regulates the employers.¹⁴⁸

However, there is a Memorandum of Understanding between the two agencies in order to share relevant information while ensuring that the exchange of such information complies with applicable law.¹⁴⁹

¹⁴⁴ Source: FDA (2018), [MOU 225-14-0002](#), retrieved on 08.01.2019

¹⁴⁵ Source: FDA (2018), [MOU 225-14-0002](#), retrieved on 08.01.2019

¹⁴⁶ Source: CPSC (2018), [Products Under the Jurisdiction of Other Federal Agencies and Federal Links](#), retrieved on 08.01.2019

¹⁴⁷ Source: OSHA (2018), [The Occupational Safety and Health Administration](#), retrieved on 08.01.2019

¹⁴⁸ Source: OSHA (2018), [1910 Subpart S](#), retrieved on 08.01.2019

¹⁴⁹ Source: OSHA (2018), [The Occupational Safety and Health Administration](#), retrieved on 08.01.2019

2.2.2.2. State level

While most of the time manufacturers focus their regulatory resources on compliance with federal requirements by the FDA, a significant portion of device regulation falls within the purview of state agencies, particularly with respect to device distribution.

In terms of device distribution, regulations are set by the state Board of Pharmacy or Board of Wholesale Distributors. Some states utilize an FDA-like agency, while others have multiple agencies that share the responsibilities in this area.¹⁵⁰

2.3. Medical device reimbursement

Reimbursement and payment are key factors in determining sales growth and market adoption. Medical communication, reimbursement, and continued compliance with regulatory requirements are particularly essential for a successful sale and distribution of medical devices.

With regard to device manufacturers that obtain reimbursement for their product, consideration must be given to the Sunshine Act.¹⁵¹

2.3.1. Sunshine Act

The Sunshine Act requires manufacturers of drugs, medical devices and biologicals participating in U.S federal health care programs to track and then report certain payments and items of value (gifts) given to physicians and teaching hospitals. Those parties are defined as "Covered Recipients". Physicians, in terms of the Sunshine Act, are any of the following types of professionals who are legally authorized to practice: Doctor of Medicine, Doctor of Osteopathy, Doctor of Dentistry and Doctor of Dental Surgery. The report has to be sent to the Centers for Medicare and Medicaid Services (CMS) on a yearly basis. The data is then published annually in a publicly searchable database.¹⁵²

Financial relationships between physicians and medical product manufacturers are common and are often a key component in the development of new drugs and devices. While these relationships can have positive aspects to it, they also do create conflicts of interests and can even blur the line between promotional activities and the conduct of medical research, training, and practice.¹⁵³

¹⁵⁰ Source: MorganLewis (2015), [State Regulation of Medical Device Distribution Update](#), retrieved on 09.01.2019

¹⁵¹ Source: NAMSA (N.A.), [Planning for Successful Medical Device Reimbursement](#), retrieved on 10.01.2019

¹⁵² Source: Celgene (2018), [Sunshine Act FAQ](#), retrieved on 09.01.2019

¹⁵³ Source: Health Affairs (2014), [The Physician Payments Sunshine Act](#), retrieved on 08.01.2019

Examples are the cost of meals provided to physicians, payments made to Covered Recipients in exchange for services provided, such as advisory boards, speaker programs and consulting engagements. Travel and provision of reprints of medical journal articles to Covered Recipients are also subject to the Act.¹⁵⁴

Companies in the research and development phase for devices not approved or cleared by the FDA may not be subject to the Sunshine Act.¹⁵⁵

Regarding a value limitation, a report is only required if an individual physician receives a single payment in excess of \$10 or exceeds \$100 in payments per year from an individual manufacturer.¹⁵⁶

However, payments or individual gifts are not prohibited. The purpose of the Act is to identify inappropriate behavior by tracking the payments and also making them accessible to the public. Furthermore, the Act does not replace state disclosure and transparency laws. So far, there is no analysis whether the Act has resulted in a reduction of financial influence of manufacturers over healthcare providers, says expert Mariana del Rio Kostenwein.¹⁵⁷

2.3.2. Coverage, Coding and Payment

Coverage, Coding and Payment are the three pillars of reimbursement and each one stands alone.¹⁵⁸

Coverage: Coverage refers to a payor's decision to provide program benefits for a specific product or service. This coverage is usually conditional on FDA clearance, the product not being deemed experimental or investigational, the medical necessity of the product, and the appropriateness of the product's use for the patient in the treatment setting.¹⁵⁹

Coverage via National Coverage Decision (NCD) or a Local Coverage Decision only applies to new medical procedures and technologies that are not currently defined in the regulations. An NCD applies only to a fraction of new devices and requires significant amount of clinical data.

The different emphasis placed on approvals by the FDA and the requirements for reimbursement by insurance companies poses a change to companies. Insurance requirements typically follow CMS guidelines. The FDA stresses safety and efficiency while the CMS focuses on superiority of a product as a main criterion. This difference makes it challenging to achieve both clearance

¹⁵⁴ Source: Celgene (2018), [Sunshine Act FAQ](#), retrieved on 09.01.2019

¹⁵⁵ Source: NAMS (N.A.), [Planning for Successful Medical Device Reimbursement](#), retrieved on 10.01.2019

¹⁵⁶ Source: Rx Vanatage, <https://www.rxvantage.com/sunshine-act/>.

¹⁵⁷ Interview with Marina del Rio Kostenwein, Partner at Simon Gluck & Kane LLP, on 08.01.2019

¹⁵⁸ Source: NAMS (N.A.), [Planning for Successful Medical Device Reimbursement](#), retrieved on 10.01.2019

¹⁵⁹ Source: The Atticus Group (2018), [Understanding Reimbursement for Medical Devices: Coding, Coverage, Payment and Payers](#), retrieved on 10.01.2019

and coverage, with the FDA making decisions on a predicate device and CMS looking for novelty.¹⁶⁰

Coding: Coding translates into payment, making it the link between coverage and payment. A proper code is necessary in order for procedures and products being paid for. The type of code varies. There are numerous of types depending on where and by whom the procedure is being performed as well as the equipment involved. Coding is often the focus of reimbursement analysis for cleared products.¹⁶¹

Payment: The amount a hospital or physician practice will get paid for a certain product determines sales; it is the reward for all effort that it took to get the product approved.

Many devices are used as part of inpatient or outpatient procedures that are covered by a single payment to the hospital for a procedure. Hospital systems are expected to provide their services at a lower cost while improving quality. Companies can often create a value proposition for direct purchase of devices that reduces length of stay, readmission and procedure time.¹⁶²

2.3.3. Centers for Medicare & Medicaid Services (CMS)

The Centers for Medicare and Medicaid Services (CMS) provide health coverage through Medicare, Medicaid, Children's Health Insurance Program and the Health Insurance Marketplace.¹⁶³

For a medical device manufacturer, it is essential to achieve CMS coverage in order demonstrate clinical and economic value for reimbursement. Medicare coverage decisions are made through CMS's National Coverage Determination (NCD) process. This program is intended to ensure prompt and efficient patient access to safe, effective and appropriate medical devices for the Medicare population.¹⁶⁴

CMS (as well as private payors, hospitals, physicians, etc.) expect data to be presented in the form of journal publications in order to review the new medical device. The publication of data should be planned early in the product development process.

A relationship between physicians and medical device companies is of high importance but also creates additional regulatory considerations once a device

¹⁶⁰ Source: NAMSA (N.A.), [Planning for Successful Medical Device Reimbursement](#), retrieved on 10.01.2019

¹⁶¹ Source: NAMSA (N.A.), [Planning for Successful Medical Device Reimbursement](#), retrieved on 10.01.2019

¹⁶² Source: NAMSA (N.A.), [Planning for Successful Medical Device Reimbursement](#), retrieved on 10.01.2019

¹⁶³ Source: USgov (2018), [Centers for Medicare and Medicaid Services](#), retrieved on 08.01.2019

¹⁶⁴ Source: Policy & Medicine (2018), [Medical Device Parallel Review Program Made Permanent](#), retrieved on 09.01.2019

is cleared for sale. Within the medical community the device needs to be accepted in order to drive sales. The best way to achieve such acceptance is by having the product presented at medical society meetings.¹⁶⁵

¹⁶⁵ Source: NAMSA (N.A.), [Planning for Successful Medical Device Reimbursement](#), retrieved on 10.01.2019

3. Market access

3.1. Market opportunities for foreign companies in the US-MedTech Industry

The continuous globalization of the US-MedTech industry is projected to surge in the future, providing promising market opportunities for foreign companies.

The industry performed well over the past five years considering the industries high-margin, strong competition and the fact that it produced mainly non-discretionary products. However, revenue decreased at the beginning of last year due to small profit margins of hospitals, which limited the ability to raise capital for large purchases. Revenue in 2018 was forecasted with a growth of 2.7% to 39.5 billion US\$. Industry growth is supported by an aging population, the expansion of healthcare coverage and technological progress. Furthermore, economic prosperity has also stimulated more consumers to seek medical care, leading to increased spending on healthcare with an annual growth rate of 3.5% over the past five years.

Compared to previous generations, baby boomers in general have a higher interest in taking care of their own healthcare due to better finances, education and wellness engagement. They are also interested in patient focused, in-home care for diabetes, heart disease and other chronic conditions. Advances in technology are expected to meet the demand of home medical devices, with the ability to quickly and easily connect to a healthcare provider's electronic records.

Drivers, such as healthcare reform, technological progress, outsourcing, regulations and the aging population, which have pushed the industry over the past five years, are expected to continue. The collective outcome of these various factors is expected to boost revenue growth at a rate of 3.0% annually to a total of 45.8 billion US\$ in 2023. Additionally, the change in US demographics is also in favor of the industry.

It is expected that small and medium sized companies are will target niche markets with the focus on one or two medical devices. Thus, the number of players in the industry is anticipated to rise over the next years to 2023.

According to IBISWorld¹⁶⁶ the following key success factors are the most important for businesses in this industry:

¹⁶⁶ Source: IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

- **Access to highly skilled workforce**

Due to the fact that the design and production of medical devices is highly technical, companies and organizations with access to skilled staff have a competitive advantage. The significance of a skilled workforce can be reflected in the industry's high average wage.

- **Access to the latest technology**

It is also very important that companies have access to the latest technology. This can be accomplished by investing in R&D or the acquisition of other enterprises that hold patented technologies.

- **Establishment of export markets**

Another key to success for a company is to operate globally. Therefore, it is important to also focus on a global expansion to develop export markets and not to solely rely on the domestic market.

- **Economies of scale**

Companies that operate large manufacturing facilities also should reduce variable costs and sales prices while monitoring to profit margins.

- **Having contacts within key markets**

It is also important to have access to distributors and end users in order to successfully sell products.

Although US companies have a tendency to dominate the industry, the expansion of international giants shows that industry profits are generated more through global outreach efforts, especially in China, Japan and Europe.

The medtech industry consists of a substantial number of foreign players that operate subsidiaries and facilities in the US. The industry is also consolidating and reaching out to emerging markets for sales. One example is the acquisition of Covidien by Medtronic in 2015.

3.2. Market barriers

Companies are often not in the position to lead in price negotiations due to big purchasing groups that act as distributors for about half of the hospitals in the US (see chapter 1.1.8. Key Distributors). Most of the larger manufacturers trust purchasing groups with the distribution of their products. Therefore, small and medium sized medical device and supply companies are excluded from sales to hospitals since the bigger players often secure exclusive contracts with purchasing groups.¹⁶⁷

¹⁶⁷ Source: IBISWorld, Medical Device Manufacturing in the US, [Medical Device Manufacturing in the US Industry Report](#), retrieved on 18.01.2019

The high average profit margins of the medical device manufacturing industry may increase the interest of potential industry participants, but there are several market entry barriers that should be considered and that may hinder industry entry. These include heavy regulation, high investment costs, large competition and the fast pace of technological progress. Most products of this industry are manufactured under patents. As a result, companies are very protective of their technological expertise and intellectual property. Industry operators who are trying to enter certain industry markets may experience demanding technical requirements with limited access to technical information. Thus, companies that are interested in competing in specialized products probably have to invest a significant amount of resources in research and development.

An additional market entry barrier may come with certain government policies. In the US medical devices are regulated by the Federal Food Drug & Cosmetic Act. Every company is required to comply with their regulations regarding medical devices. This control mechanism is the baseline requirement which applies to all devices that are needed for marketing, proper labeling and monitoring. (see chapter 2. Regulatory affairs).¹⁶⁸

Barriers to market entry checklist:

Competition	High
Concentration	High
Life Cycle Stage	Growth
Capital Intensity	Low
Technology Change	High
Regulation & Policy	Heavy
Industry Assistance	Medium

Source: IBISWorld, Medical Device Manufacturing in the US

Additionally, fees for insurances to protect against product liability claims may also discourage market entry. Especially in the field of healthcare, claims could result in prohibitively high costs with an upward trend. Another barrier is represented by the access to a very skilled labor force in order to perform high-level R&D. Very skilled and specialized labor is limited in this industry.¹⁶⁹

In general, it can be stated that the barriers to entry of the US MedTech industry are medium and steady, although it is often necessary to adapt products to the market, due to differences in needs and expectations between consumers from different cultures. This not only affects the products themselves, but also marketing strategies.

¹⁶⁸ Source: IBISWorld, Medical Device Manufacturing in the US, [Medical Device Manufacturing in the US Industry Report](#), retrieved on 18.01.2019

¹⁶⁹ Source: IBISWorld, Medical Device Manufacturing in the US, [Medical Device Manufacturing in the US Industry Report](#), retrieved on 18.01.2019

Often European entrepreneurs are more interested in technical details and tend to analyze all contingencies and possibilities before making a decision. Americans are principally more pragmatic and make decisions more instinctively. In general, it can be stated that facts are more important for European entrepreneurs, whereas their American counterparts find the presentation of the products more important.

Apart from the cultural aspects, the US also differs in terms of contract and liability law, as well as technical standards compared to Europe. In addition, legal regulations and standards may differ among the 50 US states. Companies planning to become active in the American market should obtain comprehensive information on regional and national legal and technical regulations, in order to minimize liability and recourse risks in advance. Furthermore, individual and consumer protections are much more significant in the US as opposed to in Europe.

3.3. Sales structure and market entry strategies

There are various strategic opportunities for foreign companies to start and sustain sales activities in the US. The two most common types are distribution through sales representatives and direct sales with own employees. Regardless of the chosen distribution strategy, the objectives and roles of all parties should be clearly defined when entering into a contract. Also relevant is the potential US customer.

After analyzing the market and deriving an appropriate entry strategy, it is important to address the second milestone – how to build business contacts – unless it has already been done in parallel to market research and analysis. In this phase, personal contacts are often crucial. It is recommended that these contacts be linked, constructed and/or expanded via local trade fairs and/or event participation. The appearance of a European company at trade fairs or other events also conveys a genuine interest in the US market and the search for business partners.

According to AHK USA's experience, it is imperative for foreign companies to have a presence (virtually or physically on site) in the American market in order to make market entry and expansion more effective.

It is also very important to tailor and adapt the marketing concept to the needs of the US market. This includes e.g. the communication of the "Value Added Proposition" or the unique selling points of the product or service in meaningful information material. For European products and services, the advantages over comparable American products or services should be clear. The focus should be on the customer benefit (e.g., health benefit, time or cost savings), not on the procedure or technical details. Furthermore, it should be considered that the marketing effort in the US can sometimes be more intense, requiring a larger marketing budget than in the domestic market.

3.3.1. Sales Channels

3.3.1.1. Direct Sales

Although direct selling is often the best strategy for long-term success, local distributors can drive market entry in addition to the sales representatives of their own company. Because of the size and diversity of the country, direct selling and distribution through partners can often be combined to cover different regions of the US. Basically, there are several types of distribution partners in the US, including sales agents and distributors. In principle, it should be noted that direct and indirect sales in the US are not mutually exclusive. It must be individually reviewed which strategy a company wants to utilize in the long term. Very often, the US is divided into different sales regions, which are indirectly supported by the company and partly by the local partners.

3.3.1.2. Sales Representative & Distributor

The "Sales Representative" in the USA, places orders for a commission but does not have the authority to conclude contracts on his own. Thus, the sale of the goods takes place in the name and for the account of the European company. If the commercial agent succeeds, their contracts usually are resolvable at short notice thus minimizing business risk. As part of this distribution model, however, the entire responsibility for transport, service, repair, collection and product liability usually rests with European company. A sales representative often serves a specific geographic region that can span from one city to several states. In the case of an offer intended to cover large-area territories within the USA, it is advisable to check in advance whether the agency can map a sufficient network in the entire target region and indeed has suitable contacts with the desired clientele. Basically, the cost of a sales representative is lower than that of own personnel in the US market. Some sales representatives charge a monthly fee for their services, called "Territory Development Fees" or "Retained Service Fees". However, since most of the US is commission-based, products with long sales cycles are rarely sold successfully by sales representatives.

In contrast to sales representatives, distributors directly buy the products and goods and then sell them under their own name. As a result, the distributor also assumes the risks of selling and is additionally responsible for the service after the sale of the product. Distributors can facilitate the sale and, in particular, the service for products in different regions. Especially in a large country like the US, it is necessary to

provide service in different states and regions. An advantage of working with distributors is that the business risks (except product liability and intellectual property) are with the distributor. The distributor has an interest in promoting the sale and usually has an appropriate distribution network. The disadvantage is that customers are often unknown to the European company. Also, the risk exists that additionally competing products are distributed within the same portfolio.

3.3.1.3. Group Purchasing Organizations for hospitals (GPOs)

Group Purchasing Organizations are playing a large role in the medtech industry. GPOs are organizations which have the task to assist healthcare providers to help to save costs and to become more efficient. This is done by combining purchasing power in order to negotiate discounts with industry operators that provide healthcare, e.g. manufacturers, distributors and other healthcare companies. In the US approximately 96-98% of the hospitals belong to at least one GPO, whereas a typical hospital will use two GPOs amongst the 600 GPOs US-wide. It can be said, that about 72 percent of the hospital purchases in the US are carried out by using GPO contracts with approximately 10 to 15 percent cost saving by using a GPO.¹⁷⁰

One of the reasons why GPOs have become more dominant is the shift from private practices to large hospitals. GPOs acting as the institution's administration take a larger role in the purchasing decision. This change in the buying decision of devices from physicians to administrators has shifted the focus to cost and value considered purchasing. Additionally, reimbursement usually favors larger-tier medical device manufacturers. GPOs are able to take advantage of value propositions and product differentiation towards bigger, more cost-conservative buying organizations and insurers. As a result, GPOs have replaced private practices as the main decision makers in the procurement of medical devices, which creates a barrier for smaller manufacturers and continues to prioritize value based, as well as bigger medical device companies. The following trends can be observed:

- Larger manufacturers acquiring smaller competitors to expand market share
- Hospitals undergoing corporate realignments, hindering entrance of smaller manufacturers
- Increased focus on cost-savings in hospitals
- Pricing pressures from GPOs, Medicare and other large private payers
- Higher focus on reimbursement and pricing for smaller manufacturers earlier in product development cycles

¹⁷⁰ Source: Business Sweden (N.A.), [The U.S. Medical Device Industry](#), retrieved on 16.01.2018

The process of selling to GPOs can be competitive and time consuming, especially when the bidding and review process is lengthy and can take from three months up to a year. Usually, GPOs use a bid calendar that outlines the purchase cycles and shows which product category will be procured. The determined parameter that GPOs utilize is similar to the ones that are important to hospital executives, which are high quality at the lowest possible cost (high value for money). In addition, the vendor's distribution infrastructure will be examined to make sure that high volume purchase orders can be handled properly. Lastly, vendor financials and quality services, as well as field support, are being looked at as well.

There are several steps that should be followed if a company considers selling to GPOs. The first step should be the vendor's registration with a selected GPO. The GPOs will publish a bid calendar outlining the procurement plan throughout the year which allows vendors to plan when they should approach GPOs. Business opportunities are offered by the GPOs through Request-for-Proposals (RFP) which will be forwarded to registered suppliers. After receipt of all proposals, the GPO starts to analyze each proposal and further negotiates contracts with vendors before a contract will be awarded.¹⁷¹

The following steps should be considered when selling to GPOs:

- Supplier registration
- GPO issues bid calendar for procurement categories
- Supplier registers for RFP or GPO issues RFP to list of applicable registered suppliers
- GPO analyzes proposals and products
- Negotiations between suppliers and GPOs
- GPO awards contract

Further information on GPOs can be found on the website of [Healthcare Supply Chain Association \(HSCA\)](#)¹⁷²

3.3.2. Presence in the USA

It is particularly important to show local presence in the USA. Due to the potential language barrier and time difference, it can be considered an obstacle if a European company does not have a local address and phone number in the US. Customer service is very important in the US and therefore needs to be done locally in the local language. As soon as a US market presence in the form of a subsidiary or even in the form of an address and telephone number (virtual

¹⁷¹ Source: Business Sweden (N.A.), [The U.S. Medical Device Industry](#), retrieved on 16.01.2018

¹⁷² Source: Healthcare Supply Chain Association (HSCA), [group purchasing organization \(GPO\)](#), retrieved on 18.01.2019

office / "business presence") is present, the sales opportunities for foreign companies often increase significantly.

It is also important to note that although the US is a country, there are 50 states with different state and local regulations. It is therefore highly recommended - especially at the beginning of market entry - to choose a region and then, as soon as the company is consolidated in the regional market, to expand further. For the selection of the region in which to start, it is recommended to carry out a detailed market research on supply and demand as well as the involved stakeholders etc.

In addition, the topic of personnel allocation should already be on the agenda at the beginning. Cultural differences show that Europeans tend to do very detailed planning, calculations etc. This speaks for the quality of European products, but is not effective for a marketing strategy in the US. It is therefore advisable to seek a mix of US-Americans and own nationals in the search for personnel.

However, for a foreign company with substantial activities in the US it is advisable and necessary to set up a presence in the US. Determining the way of setting up such presence depends on many different aspects within the business.

In general, there are two main options: 1) Virtual or 2) Physical office. Both types are sufficient to run a branch office or as headquarter for an US - subsidiary.

A virtual office is a virtual office environment with the benefits of an US business address. For example, the virtual office services offered by the GACC New York include establishing a company's personalized mailing address and phone line in Manhattan's Financial District at an affordable price. Specially trained, bilingual employees in our consulting department manage incoming and outgoing correspondence and answer calls on behalf of the company. However, there are numerous other service providers in the US that offer a similar service, e.g. Regus¹⁷³ or Servcorp¹⁷⁴.

The main question is, however, whether to form a branch or a subsidiary when considering opening a presence. The liabilities and financial impacts vary significant. Whereas a branch exposes the company's entire earnings, an incorporated subsidiary limits this kind of financial exposure.¹⁷⁵

Moreover, companies need to take into account that a US company corporation is administered at the state level (state law, federal law only being applicable occasionally); therefore, the process does differ from state to state.¹⁷⁶

¹⁷³ Source: [Regus](#)

¹⁷⁴ Source: [Servcorp](#)

¹⁷⁵ Source: GACC brochure „Firmengruendung in den USA“

¹⁷⁶ Source: GACC brochure „Firmengruendung in den USA“

3. 3. 2. 1. Branch

A branch office does not constitute a separate legal entity of the parent company, but is an unincorporated extension of a foreign parent company operating a sales office or other income producing activity in the US.¹⁷⁷ However, due to this structure the parent company is fully exposed to any and all business risk inherent in doing business in the US. This option is therefore not chosen very often.¹⁷⁸

3. 3. 2. 2. Subsidiary / US Legal Entity

A subsidiary is a separate legal entity from the parent company, but still owned by the parent company. It can be formed as any type of legal entity; the most common forms are corporations and limited liability companies.¹⁷⁹ Most foreign companies choose to set up a corporation since it can be established quickly, only requiring minimal administrative burden. Furthermore, it allows a centralized management as well as limitation of liability.¹⁸⁰

There are mainly four types of companies in the United States: General Corporation (C Corporation), S Corporation, Close Corporation, Limited Liability Company (LLC). Each form has advantages and disadvantages in complexity, ease of setup, cost, liability protection, periodic reporting requirements, operating complexity, and taxation.

A General Corporation (or "C Corporation") is the most common corporate structure for medium and large companies. An S Corporation is actually a C Corporation which then obtains a special tax status from the Internal Revenue Service (IRS). Both C and S Corporations offer limited liability protection. Both require articles of incorporation to be filed. And both comprise shareholders, directors, and officers. There are lots of similarities, but they differ in the complex realm of taxation and corporate ownership.

C corporations are subject to double taxation while S corporations are pass-through tax entities, allowing them to avoid being taxed at the corporate level and again on shareholders' personal income taxes. C corporations have no restriction on ownership, S corporations are restricted to no more than 100 shareholders who must be US citizens or residents.

A Close Corporation is similar to a C Corporation, except the number of shareholders is limited to 30, the transfer of shares is conditional to the

¹⁷⁷ Source: [US Branch Office](#)

¹⁷⁸ Source: [US Branch Office](#)

¹⁷⁹ Source: [US Branch Office](#)

¹⁸⁰ Source: GACC brochure „Firmengruendung in den USA“

directors' prior approval and the prohibition to trade shares on the stock exchange.

A Limited Liability Company (LLC) is formed by one or more individuals or entities through a special written agreement. Unlike an S corporation or C corporation, the structure of an LLC is flexible. The LLC business structure combines the pass-through taxation of a partnership or sole proprietorship with the limited liability of a corporation.

In order to set up a business in the US, following steps should be considered:

1. Choosing which type of business entity to form: Corporation or LLC

If any of the company owners (called "Shareholders" for corporations and "Members" for LLC's) are not US Citizens, then either a Corporation or an LLC can be formed.

2. Choosing in which state to form the Corporation or LLC

In the United States, you can form a Corporation or LLC in any of the 50 States. Some US-States are more "business-friendly" or "international-friendly" than others (e.g. Delaware).

3. Designating a registered agent

The Registered Agent has a statutory responsibility to accept official state documents and legal documents and forward them to the company.

4. Providing names and addresses of the people/companies involved (Officers, directors, members, etc.)

5. Acquiring an EIN

The Federal Employer Identification Number (FEIN) also known as an "EIN" or simply "Tax ID Number" is a number issued by the United States Internal Revenue Service (IRS) that is somewhat like an identification number for companies. It allows you to open bank accounts, pay taxes and hire employees.

The German American Chamber of Commerce, Inc. can provide support in setting up a legal entity in the United States.¹⁸¹

¹⁸¹ Source: GACC brochure „Firmengruendung in den USA“

Having a permanent, incorporated subsidiary in the US has several benefits: The parent company will be protected from potential liabilities in the US. Additionally, it will simplify bookkeeping and accounting, making tax compliance less costly and more efficient, being able to cover insurance and to open a bank account. The subsidiary can also be qualified as a local company when bidding on certain contracts.¹⁸²

For further information please contact:

German American Chamber of Commerce, Inc.
80 Pine Street, Floor 24 | New York, NY 10005
Phone: (212) 974-8846 | Fax: (212) 974-8867
E-Mail: legalservices@gaccny.com
URL: www.gaccny.com | www.ahk-usa.com | www.ahk.de

¹⁸² Source: GTAI (2018), [Unternehmensgründung und Gewerbeanmeldung in USA](#), retrieved on 08.01.2019

List of Sources

APAO (2019), [Oncology Professional Organizations](#), retrieved on 18.01.2019
 Business Sweden (N.A.), [The U.S. Medical Device Industry](#), retrieved on 16.01.2018
 CBP, [Customs Duty Information](#), retrieved on 08.01.2019
 Celgene (2018), [Sunshine Act FAQ](#), retrieved on 09.01.2019
 CPSC (2018), [Products Under the Jurisdiction of Other Federal Agencies and Federal Links](#), retrieved on 08.01.2019
[Device Registration and Listing](#), retrieved on 08.01.2019
 European Commission (2018), [Dual-use trade controls](#), retrieved on 10.01.2019
 EY (2016), [Pulse of the Industry](#), retrieved on 13.12.2018
 FDA (1997), [Design Control Guidance for Medical Device Manufacturers](#), retrieved on 08.01.2019
 FDA (2018), [510\(k\) Clearances](#), retrieved on 10.01.2019
 FDA (2018), [CBER Regulated Products](#), retrieved on 08.01.2019
 FDA (2018), [Classify Your Medical Device](#), retrieved on 10.01.2019
 FDA (2018), [Code of Federal Regulations \(CFR\)](#), retrieved on 16.01.2019
 FDA (2018), [Device Advice: Comprehensive Regulatory Assistance](#), retrieved on 08.01.2019
 FDA (2018), [Device Advice: Investigational Device Exemption \(IDE\)](#), retrieved on 08.01.2019
 FDA (2018), [Device Classification Panels](#), retrieved on 08.01.2019
 FDA (2018), [Device Labeling](#), retrieved on 10.08.2019
 FDA (2018), [Evaluation of Automatic Class III Designation \(De Novo\)](#), retrieved on 08.01.2019
 FDA (2018), [General Controls for Medical Devices](#), retrieved on 09.01.2019
 FDA (2018), [General Device Labeling Requirements](#), retrieved on 08.01.2019
 FDA (2018), [Guidance for Industry and Food and Drug Administration Staff](#), retrieved on 18.01.2019
 FDA (2018), [How to Study and Market Your Device](#), retrieved on 07.01.2019
 FDA (2018), [How to Study and Market Your Device](#), retrieved on 17.01.2019
 FDA (2018), [Humanitarian Device Exemption](#), retrieved on 08.01.2019
 FDA (2018), [Important Reminders about Registration and Listing](#), retrieved on 09.01.2019
 FDA (2018), [Importing into the U.S.](#), retrieved on 10.01.2019
 FDA (2018), [Importing into the U.S.](#), retrieved on 10.01.2019
 FDA (2018), [Mandatory Reporting Requirements: Manufacturers, Importers and Device User Facilities](#), retrieved on 08.01.2019
 FDA (2018), [Medical Device Accessories](#), retrieved on 09.01.2019
 FDA (2018), [Medical Device Reporting \(MDR\)](#), retrieved on 10.01.2019
 FDA (2018), [MOU 225-14-0002](#), retrieved on 08.01.2019
 FDA (2018), [Oncology Devices and Diagnostics](#), retrieved on 18.01.2019
 FDA (2018), [Overview of Device Regulation](#), retrieved on 27.01.2018
 FDA (2018), [Payment Process](#), retrieved on 09.01.2019
 FDA (2018), [PMA Approvals](#), retrieved on 08.01.2019
 FDA (2018), [Premarket Approval \(PMA\)](#), retrieved on 09.01.2019
 FDA (2018), [Premarket Notification 510\(k\)](#), retrieved on 08.01.2019
 FDA (2018), [Products and Medical Procedures](#), retrieved on 08.01.2019
 FDA (2018), [Quality System \(QS\) Regulation/Medical Device Good Manufacturing Practices](#), retrieved on 08.01.2019
 FDA (2018), [What is the difference between the Federal Food, Drug, and Cosmetic Act \(FD&C Act\), FDA regulations, and FDA guidance?](#), retrieved on 17.01.2019
 FDA (2018), [Who Must Register, List and Pay the Fee](#), retrieved on 08.01.2019
 Focus Economics (2018), [United States Economy Overview](#), retrieved on 13.12.2018
 GACC brochure „Firmengruendung in den USA“
 GACC brochure „Firmengruendung in den USA“
 GACC brochure „Firmengruendung in den USA“
 GE (2018), [GE Healthcare](#), retrieved on 22.01.2019
 Global Markets Insight (2017), [Orthopedic Devices Market Size By Product](#), retrieved 18.01.2019

GovInfo (N.A.), [Federal Register Volume 61, Issue 195 \(October 7, 1996\)](#), retrieved 14.01.2019FDA (2018), [Quality System \(QS\) Regulation/Medical Device Good Manufacturing Practices](#), retrieved on 08.01.2019

GTAI (2018), [Merkblatt über gewerbliche Wareneinführen – USA](#), retrieved on 10.01.2019

GTAI (2018), [Merkblatt über gewerbliche Wareneinführen und Basiswissen Einfuhr](#), retrieved on 08.01.2019

GTAI (2018), [Merkblatt über gewerbliche Wareneinführen-USA](#), retrieved on 08.01.2019

GTAI (2018), [Unternehmensgründung und Gewerbeanmeldung in USA](#), retrieved on 08.01.2019

Health Affairs (2014), [The Physician Payments Sunshine Act](#), retrieved on 08.01.2019

Healthcare Supply Chain Association (HSCA), [group purchasing organization \(GPO\)](#), retrieved on 18.01.2019

Hoovers (2018), [Abbott Laboratories](#), retrieved on 18.01.2019

Hoovers (2018), [Abiomed](#), retrieved on 18.01.2019

Hoovers (2018), [Boston Scientific](#), retrieved on 18.01.2019

Hoovers (2018), [Depuy Synthes, Inc.](#), retrieved on 22.01.2019

Hoovers (2018), [Edwards Lifesciences](#), retrieved on 18.01.2019

Hoovers (2018), [Getinge](#), retrieved on 18.01.2019

Hoovers (2018), [Globus Medical, Inc.](#), retrieved on 18.01.2019

Hoovers (2018), [Johnson & Johnson](#), retrieved on 18.01.2019

Hoovers (2018), [Johnson & Johnson](#), retrieved on 18.01.2019

Hoovers (2018), [Medtronic](#), retrieved on 18.01.2019

Hoovers (2018), [Medtronic](#), retrieved on 18.01.2019

Hoovers (2018), [NuVasive](#), retrieved on 18.01.2019

Hoovers (2018), [Orthofix](#), retrieved on 18.01.2019

Hoovers (2018), [Stryker Corporation](#), retrieved on 18.01.2019

Hoovers (2018), [Terumo](#), retrieved on 18.01.2019

Hoovers (2018), [W.L. Gore & Associates](#), retrieved on 18.01.2019

Hoovers (2018), [Wright Medical Group](#), retrieved on 18.01.2019

Hoovers (2018), [Zimmer Biomet Holdings](#), retrieved on 18.01.2019

Hoovers (2019), [3M](#), retrieved on 14.01.2019

Hoovers (2019), [A-dec](#), retrieved on 14.01.2019

Hoovers (2019), [A-dec](#), retrieved on 14.01.2019

Hoovers (2019), [Allogene Therapeutics](#), retrieved on 14.01.2019

Hoovers (2019), [AMD Lasers](#), retrieved on 14.01.2019

Hoovers (2019), [Arthrex](#), retrieved on 14.01.2019

Hoovers (2019), [Biolase](#), retrieved on 14.01.2019

Hoovers (2019), [C.R. Bard](#), retrieved on 14.01.2019

Hoovers (2019), [Carestream Health](#), retrieved on 14.01.2019

Hoovers (2019), [Danaher Corporation](#), retrieved on 23.01.2019

Hoovers (2019), [Dentsply Sirona](#), retrieved on 14.01.2019

Hoovers (2019), [Elekta](#), retrieved on 14.01.2019

Hoovers (2019), [Flatiron Health](#), retrieved on 14.01.2019

Hoovers (2019), [Guardant Health](#), retrieved on 18.01.2019

Hoovers (2019), [Henry Schein](#), retrieved on 23.01.2019

Hoovers (2019), [Nanthealth](#), retrieved on 18.01.2019

Hoovers (2019), [Patterson Companies, Inc.](#), retrieved on 14.01.2019

Hoovers (2019), [Varian Medical Systems](#), retrieved on 18.01.2019

IBISWorld (2017), [Cardiologists Industry in the US](#), retrieved on 14.01.2019

IBISWorld (2018), [Dental Equipment Dealers Industry in the US](#), retrieved on 14.01.2019

IBISWorld (2018), [Dental Equipment Dealers Industry in the US](#), retrieved on 14.01.2019

IBISWorld (2018), [Dental Equipment Dealers Industry in the US](#), retrieved on 14.01.2019

IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

IBISWorld (2018), [Medical Device Manufacturing in the US Industry Report](#), retrieved on 16.01.2019

International Trade Administration (2016), [2016 Top Markets Report Medical Device](#), retrieved on

Interview with Marina der Rio Kostenwein, Partner at Simon Gluck& Kane LLP, on 08.01.2019

Interview with Marina der Rio Kostenwein, Partner at Simon Gluck& Kane LLP, on 08.01.2019

Interview with Marina der Rio Kostenwein, Partner at Simon Gluck& Kane LLP, on 08.01.2019

Interview with Winthrop Turlow, Executive Director of MedTech Association from 10.01.2019

Johnson & Johnson (2018), [Reported Sales vs Prior Period \(\\$MM\)](#), retrieved on 22.01.2019

Medtronic (2018), [Facts and Statistics](#), retrieved on 14.01.2019

MorganLewis (2015), [State Regulation of Medical Device Distribution Update](#), retrieved on 09.01.2019

NAMSA (N.A.), [Planning for Successful Medical Device Reimbursement](#), retrieved on 10.01.2019

NAMSA (N.A.), [Planning for Successful Medical Device Reimbursement](#), retrieved on 10.01.2019

National Academies Press (US), [A Nationwide Framework for Surveillance of Cardiovascular and Chronic Lung Diseases](#), retrieved on 18.01.2019

National Cancer Institute (2018), [Cancer State](#), retrieved on 18.01.2019

National Cancer Institute (2018), [Cancer State](#), retrieved on 18.01.2019

OSHA (2018), [1910 Subpart S](#), retrieved on 08.01.2019

OSHA (2018), [The Occupational Safety and Health Administration](#), retrieved on 08.01.2019

Policy & Medicine (2018), [Medical Device Parallel Review Program Made Permanent](#), retrieved on 09.01.2019

[Regus](#)

Rx Vanatage, <https://www.rxvantage.com/sunshine-act/.Servcom>

Source: Statista (2018), [Distribution of Medtronic's revenue from 2014 to 2018, by segment \(in million U.S. dollars\)](#), retrieved 14.01.2019

Statista (2016), [North America's dental equipment market size from 2012 to 2020, by product \(in million U.S. dollars\)](#), retrieved on 17.01.2019

Statista (2017), [Global top 10 companies based on cardiologic medical technology market share in 2017 and 2024](#), retrieved on 09.01.2019

Statista (2017), [Top 20 companies based on medical technology R&D spending worldwide in 2017 and 2014 \(in million U.S. dollars\)](#), retrieved on 9.01.2019

Statista (2018) [Medical technology industry](#), retrieved on 03.01.2019

Statista (2018) [Medical technology industry](#), retrieved on 03.01.2019

Statista (2018), [Global top 10 companies based on orthopedic medical technology market share in 2017 and 2024](#), retrieved on 18.01.2019

Statista (2018), [Leading U.S. medtech regions](#), retrieved on 12.12.2018

Statista (2018), [Oncology](#), retrieved on 17.12.2018

Statista (2018), [Share of Americans who underwent orthopedic treatment in the last 3 years in 2018, by age](#), retrieved on 18.01.2019

The Atticus Group (2018), [Understanding Reimbursement for Medical Devices: Coding, Coverage, Payment and Payers](#), retrieved on 10.01.2019

Transparency Market Research (2018), [Oncology Devices Market](#), retrieved on 15.01.2019

United States Census Bureau (2018): [Quick Facts United States](#) und [U.S International Trade in Goods and Services](#), retrieved on 13.12.2018

[US Branch Office](#)

USgov (2018), [Centers for Medicare and Medicaid Services](#), retrieved on 08.01.2019

USgov (2018), [Importing and Exporting](#), retrieved on 08.01.2019

USTR (2018), [United States-Mexico-Canada Agreement](#), retrieved on 08.01.2019

Wiley Online Library (2018), [Cancer Statistics 2018](#), retrieved on 23.01.2019

[Wireless Medical Devices](#), retrieved on 08.01.2019

Zoll, [Wirtschaft und Sicherheit](#), retrieved on 10.01.2018.